

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

MAY 07 2009

Supervisor/Operator Performing the Verification Procedure: DataMaster cdm S/N 130567 ✓

Name DEREK A MCGARRIGAN ID# 5420 Date 5/1/09 ✓

A Agency KETCHIKAN POLICE DEPARTMENT Phone # 225-6631

Instrument Location KTN. POLICE DEPARTMENT, 361 MAIN ST., KETCHIKAN AK 99901

B Alco S/N X301568 ✓ Target Value .080 ✓ High Pressure 500

Alco Test Value Average .087 ✓ .088 ✓
1st Alco 2nd Alco

Signature [Signature] ✓

[Signature]
5/13/09

(OVER)

(Do Not write in the area below)


I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the

[Signature]
Nita J. Bolz
Scientific Director
State Breath Alcohol Program

Subscribed and sworn before me this 22 day of May 2009.

[Signature] (Notary Seal Stamp)
Carolyn M. Noland
Notary Public, State of Alaska
Commission Expires with Office



VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska


Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130567

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

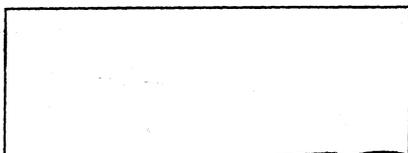

ALCOHOL METER SAFETY
DATA MASTER cdm 130567

MAY 01, 2009 ✓

OPERATOR'S NAME:

MCARRIGAN BEREK A

OPERATOR'S NUMBER: 5420

SUBJECT'S LAST NAME:

VOC

SUBJECT'S FIRST NAME/MI :

VOC

O.L. #: 1234567

DEPT/AGENCY: KET1

CASE/REPORT: 09-1

TEST TYPE: V


ALCO TARGET VALUE: .000 ✓

ALCO S/N: X301568

--- BREATH ANALYSIS ---

.000 ADJUSTED FOR 30.11 in		
ALCO TARGET	.000	17:13
BLANK TEST	.000	17:14
INTERNAL STANDARD	VERIFIED	17:14
ALCO TV 30.11 in	.007 ✓	17:14
BLANK TEST	.000	17:15
SUBJECT SAMPLE	.000	17:16
BLANK TEST	.000	17:17
ALCO TV 30.11 in	.000 ✓	17:17
BLANK TEST	.000	17:18

DIAGNOSTIC CHECK



ALCOHOL METER SAFETY
DATA MASTER cdm 130567

MAY 01, 2009 ✓

TIME 17:11

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY

PROGRAM: OKAY

SOFTWARE DATE: 02/20/01

HEATERS

SAMPLE CHAMBER: 50c

BREATH TUBE: 42c

BAROMETER: 30.11 in

FLOW DETECTOR: OKAY

PUMP

HIGH SPEED: OKAY

DETECTOR: OKAY

FILTERS: OKAY

QUARTZ STANDARD: OKAY

CALIBRATION: OKAY

PRINTER TEST

! " # \$ % & ' () * + , - . / 0 1 2 3 4 5 6 7 8 9 : ; < = > ? @ A B C D E F G
H I J K L M N O P Q R S T U V W X Y Z [\] ^ _ ` a b c d e f g h i j k l m n o
p q r s t u v w x y z () * +