

VERIFICATION OF CALIBRATION REPORT

Of Data Master cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statedwide Breath Alcohol Program

JAN 11 2011
2011
3/1/11

Supervisor/Operator Performing the Verification Procedure:	
Name Mac Burrell	DataMaster cdm S/N 130569 ✓
ID # 4756 ✓	Date 1/4/2011 ✓
Agency Cordova Police Department	Phone # 424-6100
Instrument Location Cordova Police Department	
Alco S/N 65859 ✓ Target Value 0.081 ✓ High Pressure 1100	
Alco Test Value Average 0.079 ✓ 1st Alco	0.08 ✓ 2nd Alco
Signature <i>Mac Burrell</i>	
(OVER)	

BMB
2/8/11


- I, Nita J. Bolz, after being first duly sworn, depose and state as follows:
- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory. *(Do Not Write in the area below)*
 - (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
 - (3) I am the Scientific Director of the State Breath Alcohol Program.
 - (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
 - (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
 - (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

Nita J. Bolz
Nita J. Bolz
Scientific Director
State Breath Alcohol Program



Subscribed and sworn before me this 11th day of MAR, 2011

Daniel L. Nicholas
(Notary Seal Stamp)
Daniel L. Nicholas
Notary Public, State of Alaska
Commission Expires with Office

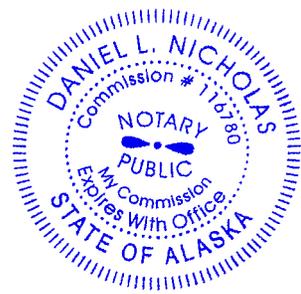

VERIFICATION OF CALIBRATION REPORT

Of Data Master cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statedwide Breath Alcohol Program

DataMaster cdm S/N

130569

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130569

JANUARY 04, 2011

OPERATOR'S NAME:

BURRELL/M

OPERATOR'S NUMBER: 175

SUBJECT'S LAST NAME:

VERIFICATION OF TIL

SUBJECT'S FIRST NAME:

A

O.L. #: A

TEST AGENCY: CDH

CASE/REPORT: 010411

TEST TYPE: V

ALCO TARGET VALUE: .081

ALCO S/N: 65859

--- BREATH TEST ---

.081 ADJUSTED FOR 29.38 in
ALCO TARGET 079 17:48
BLANK TEST 080 17:49
INTERNAL STANDARD VERIFIED 17:49
ALCO TV 29.38 in 079 17:50
BLANK TEST 080 17:51
SUBJECT SAMPLE 080 17:52
BLANK TEST 080 17:53
ALCO TV 29.38 in 080 17:53
BLANK TEST 080 17:54

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130569

JANUARY 04, 2011

TIME 17:42

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY

PROGRAM: OKAY

SOFTWARE DATE: 02/29/01

WEETERS

SAMPLE CHAMBER: 43c

BREATH TUBE: 43c

BAROMETER: 29.39 in

FLOW DETECTOR: OKAY

PUMP

HIGH SPEED: OKAY

DETECTOR: OKAY

FILTERS: OKAY

QUARTZ STANDARD: OKAY

CALIBRATION: OKAY

PRINTER TEST

!@#%&'()*+,-./0123456789:;<=>?@BCDEFG
HIJKLMNOPQRSTUVWXYZ[\]^_`{|}~:;@#%&'()*+,-./0123456789:;<=>?@BCDEFG
HIJKLMNOPQRSTUVWXYZ[\]^_`{|}~:;@#%&'()*+,-./0123456789:;<=>?@BCDEFG