

# VERIFICATION OF CALIBRATION REPORT

Of Data Master cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statedwide Breath Alcohol Program

FEB 22 2010

Supervisor/Operator Performing the Verification Procedure:	
Name <b>MAC BURRELL</b>	ID # <b>4756</b> Date <b>2/17/2010</b>
Agency <b>Cordova Police Department</b>	Phone # <b>424-6100</b>
Instrument Location <b>Cordova Police Department</b>	
DataMaster cdm S/N <b>130569</b>	
Alco S/N <b>X301686</b> Target Value <b>0.086</b> High Pressure <b>850 PSI</b>	
Alco Test Value Average <b>0.086</b> <b>0.087</b>	
1st Alco 2nd Alco	
Signature <i>Mac Burrell</i>	

(OVER)

BMB  
2/23/2010

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (Do Not write in the area below)
- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
  - (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
  - (3) I am the Scientific Director of the State Breath Alcohol Program.
  - (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
  - (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
  - (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

*Nita J. Bolz*  
Nita J. Bolz  
Scientific Director  
State Breath Alcohol Program



Subscribed and sworn before me this 24th day of February, 2010.

*Carolyn M. Noland*  
(Notary Seal Stamp)



Carolyn M. Noland  
Notary Public, State of Alaska  
Commission Expires with Office

# VERIFICATION OF CALIBRATION REPORT

Of Data Master cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statedwide Breath Alcohol Program

DataMaster cdm S/N

130569

(CONTINUED FROM FRONT PAGE)

**C** TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130569

FEBRUARY 17, 2010

OPERATOR'S NAME:

DURRELL/H

OPERATOR'S NUMBER: 4756

SUBJECT'S LAST NAME:

VERIFICATION OF CAL

SUBJECT'S FIRST NAME/MI :

L

O.L. #: L

DEPT/AGENCY: CDV1

CRSE/REPORT:

TEST TYPE: V

ALCO TARGET VALUE: .006

ALCO S/N: X001606

--- BREATH ANALYSIS ---

.006 ADJUSTED FOR 30.09 in

ALCO TARGET .006 19:40

BLANK TEST .000 19:41

INTERNAL STANDARD VERIFIED 19:41

ALCO TV 30.09 in .006 19:42

BLANK TEST .000 19:42

SUBJECT SAMPLE .000 19:43

BLANK TEST .000 19:44

ALCO TV 30.09 in .007 19:45

BLANK TEST .000 19:46

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130569

FEBRUARY 17, 2010

TIME 19:35

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY

PROGRAM: OKAY

SOFTWARE DATE: 02/20/01

HEATERS

SAMPLE CHAMBER: 49c

BREATH TUBE: 42c

BAROMETER: 30.09 in

FLOW DETECTOR: OKAY

PUMP

HIGH SPEED: OKAY

DETECTOR: OKAY

FILTERS: OKAY

QUARTZ STANDARD: OKAY

CALIBRATION: OKAY

PRINTER TEST

!"#\$%&'()\*+,-./0123456789:;<=>?@ABCDEFGHIJ  
KLMNOPQRSTUVWXYZ[\]^\_`abcde fghijklmno  
pqrstuvwxyz{|}~

# VERIFICATION OF CALIBRATION REPORT

Of Data Master cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statedwide Breath Alcohol Program

DataMaster cdm S/N

130569

(CONTINUED FROM FRONT PAGE)

**C** TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130569

FEBRUARY 17, 2010

OPERATOR'S NAME:  
BURRELL/M

OPERATOR'S NUMBER: 4756

SUBJECT'S LAST NAME:

VERIFICATION OF CAL

SUBJECT'S FIRST NAME/MI :

L

O.L. #: L

DEPT/AGENCY: CDV1

CASE/REPORT:

TEST TYPE: V

ALCO TARGET VALUE: .086

ALCO S/N: X301686

### --- BREATH ANALYSIS ---

.086 ADJUSTED FOR 30.09 in  
ALCO TARGET .086 19:40  
BLANK TEST .000 19:41  
INTERNAL STANDARD VERIFIED 19:41  
ALCO TV 30.09 in .086 19:42  
BLANK TEST .000 19:42  
SUBJECT SAMPLE .000 19:43  
BLANK TEST .000 19:44  
ALCO TV 30.09 in .087 19:45  
BLANK TEST .000 19:46

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130569

FEBRUARY 17, 2010  
TIME 19:35

### --- DIAGNOSTIC CHECK ---

COMPUTER: OKAY  
PROGRAM: OKAY  
SOFTWARE DATE: 02/20/01  
HEATERS  
SAMPLE CHAMBER: 49c  
BREATH TUBE: 42c  
BAROMETER: 30.09 in  
FLOW DETECTOR: OKAY  
PUMP  
HIGH SPEED: OKAY  
DETECTOR: OKAY  
FILTERS: OKAY  
QUARTZ STANDARD: OKAY  
CALIBRATION: OKAY

### PRINTER TEST

!"#\$%&'()\*+,-./0123456789:;<=>?@ABCDEFGHIJ  
KLMNOPQRSTUVWXYZ[\]^\_`abcdefgijklmnop  
qrstuvwxyz{|}~"

# VERIFICATION OF CALIBRATION REPORT

Of Data Master cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statedwide Breath Alcohol Program

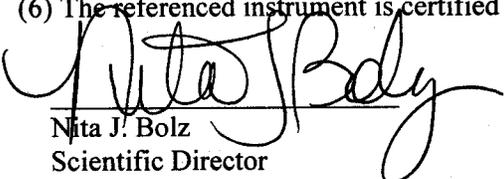
FEB 22 2010

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	130569 ✓
A	Name	MAC BURRELL	ID # 4756 Date 2/17/2010 ✓
	Agency	Cordova Police Department	Phone # 424-6100
	Instrument Location	Cordova Police Department ✓	
B	Alco S/N	X301686 ✓	Target Value 0.086 High Pressure 850 PSI
	Alco Test Value Average	0.086 ✓ 1st Alco	0.087 ✓ 2nd Alco
	Signature	Mac Burrell ✓	
(OVER)			

BMB  
2/23/2010

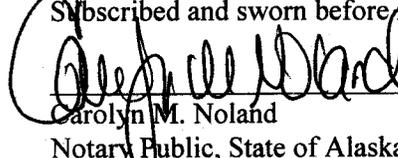
I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (Do Not write in the area below)
- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
  - (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
  - (3) I am the Scientific Director of the State Breath Alcohol Program.
  - (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
  - (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
  - (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

  
Nita J. Bolz  
Scientific Director  
State Breath Alcohol Program



Subscribed and sworn before me this 24<sup>th</sup> day of February, 2010.

  
(Notary Seal Stamp)  
Carolyn M. Noland  
Notary Public, State of Alaska  
Commission Expires with Office

