


VERIFICATION OF CALIBRATION REPORT

Of Data Master cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statedwide Breath Alcohol Program

FEB 25 2009

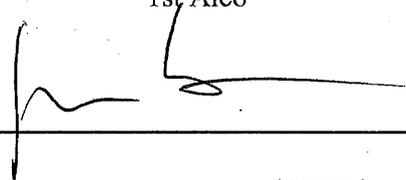		DataMaster cdm S/N	<u>130569</u>
Supervisor/Operator Performing the Verification Procedure:			
Name	<u>John Hodges</u>	ID #	<u>2999</u> Date <u>2/20/2009</u> ✓
A			
Agency	<u>Cordova Police Department</u>	Phone #	<u>424-6100</u>
Instrument Location	<u>Cordova Police Department</u>	✓	
B			
Alco S/N	<u>X124634</u> ✓	Target Value	<u>0.078</u> ✓ High Pressure <u>1000psi</u>
Alco Test Value Average	<u>0.081</u> ✓	<u>0.081</u> ✓	
	1st Alco	2nd Alco	
Signature			<u>JS</u> <u>3/2/09</u>


Under the Alaska Rules of Evidence, I certify that; (OVER)

(Do Not write in the area below)
(a) I am Jeanne Swartz, Forensic Scientist III, Scientific Crime Detection Laboratory, State of Alaska Department of Public Safety, and was, at the time of signing, the custodian of the records of the aforementioned laboratory and the signature was made in my official capacity as Scientific Director Designee of the State Breath Alcohol Testing Program.

(b) The verification of calibration for the above instrument has been received and reviewed. Instrument operator, John Hodges, whose name appears in my records, is qualified to verify the calibration of the above instrument.

(c) This instrument is certified for evidentiary use and these records are being retained as original documents in my custody.

Signed and sealed,



Jeanne Swartz
Scientific Director Designee
State of Alaska
State Breath Alcohol Testing Program

3/2/09
Date

VERIFICATION OF CALIBRATION REPORT

Of Data Master cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statedwide Breath Alcohol Program

DataMaster cdm S/N

130569 ✓

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130569

FEBRUARY 20, 2009

OPERATOR'S NAME: HODGES, JOHN
OPERATOR'S NUMBER: 2999
SUBJECT'S LAST NAME:
VERIFICATION OF CAL
SUBJECT'S FIRST NAME/MI :
X

O.L. #: X
DEPT/AGENCY: CDVI
CASE/REPORT: X
TEST TYPE: V
ALCO TARGET VALUE: .078 ✓
ALCO S/N: X124634 ✓

--- BREATH ANALYSIS ---

.078 ADJUSTED FOR 30.38 in
ALCO TARGET .078 23:35
BLANK TEST .000 23:36
INTERNAL STANDARD VERIFIED 23:36
ALCO TV 30.38 in .001 ✓ 23:37
BLANK TEST .000 23:37
SUBJECT SAMPLE .000 23:38
BLANK TEST .000 23:39
ALCO TV 30.38 in .001 ✓ 23:40
BLANK TEST .000 23:41

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130569

FEBRUARY 20, 2009 ✓
TIME 23:53

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY
PROGRAM: OKAY
SOFTWARE DATE: 02/20/01
HEATERS
SAMPLE CHAMBER: 49c
BREATH TUBE: 42c
BAROMETER: 30.38 in
FLOW DETECTOR: OKAY
PUMP
HIGH SPEED: OKAY
DETECTOR: OKAY
FILTERS: OKAY
QUARTZ STANDARD: OKAY
CALIBRATION: OKAY

PRINTER TEST

!"#\$%&'()*+,-./0123456789:;<=>?@ABCDEF6
HIJKLMNPOQRSTUVWXYZ[\]^_`abcde fghi jk lmnop
qrs;tuvwxyz{|}~`