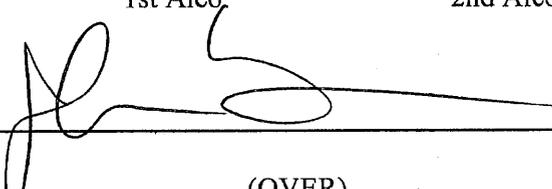


# VERIFICATION OF CALIBRATION REPORT

Of Data Master cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statedwide Breath Alcohol Program

		DataMaster cdm S/N	130569 ✓						
Supervisor/Operator Performing the Verification Procedure:									
Name		John Hodges	ID #	2999	Date	3/4/2008 ✓			
A	Agency		Cordova Police Department		Phone #	424-6100			
Instrument Location		Cordova Police Department							
Alco S/N					78853 ✓	Target Value	0.078 ✓	High Pressure	300psi
B	Alco Test Value Average		0.077	0.078					
		1st Alco.	2nd Alco						
Signature									
		(OVER)			CSB 3/10/08				

Under the Alaska Rules of Evidence, I certify that,


(Do Not write in the area below)


(a) I am Jeanne Swartz, Criminalist III, Scientific Crime Detection Laboratory, State of Alaska Department of Public Safety, and was, at the time of signing, the custodian of the records of the aforementioned laboratory and the signature was made in my official capacity as Scientific Director Designee of the State Breath Alcohol Testing Program.

(b) The verification of calibration for the above instrument has been received and reviewed. Instrument operator, John Hodges, whose name appears in my records, is qualified to verify the calibration of the above instrument.

(c) This instrument is certified for evidentiary use and these records are being retained as original documents in my custody.

Signed and sealed,

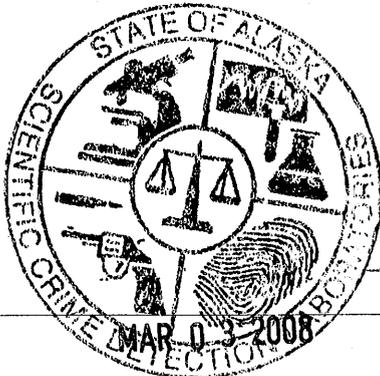



Jeanne Swartz  
Scientific Director Designee  
State of Alaska  
State Breath Alcohol Testing Program

03/10/08

Date

# VERIFICATION OF CALIBRATION REPORT

Of Data Master cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statedwide Breath Alcohol Program

DataMaster cdm S/N

130569

(CONTINUED FROM FRONT PAGE)

**C** TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130569

MARCH 04, 2008

OPERATOR'S NAME:

HODGES, JOHN

OPERATOR'S NUMBER: 2999

SUBJECT'S LAST NAME:

VERIFICATION OF CAL

SUBJECT'S FIRST NAME/MI :

X

O.L. #: X

DEPT/AGENCY: CDVI

CASE/REPORT: X

TEST TYPE: V

ALCO TARGET VALUE: .078

ALCO S/N: 78853

### --- BREATH ANALYSIS ---

.078 ADJUSTED FOR 30.30 in  
ALCO TARGET .079 19:10  
BLANK TEST .000 19:11  
INTERNAL STANDARD VERIFIED 19:11  
ALCO TV 30.30 in .077 19:11  
BLANK TEST .000 19:12  
SUBJECT SAMPLE .000 19:14  
BLANK TEST .000 19:15  
ALCO TV 30.30 in .078 19:15  
BLANK TEST .000 19:16

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130569

MARCH 04, 2008

TIME 19:17

### --- DIAGNOSTIC CHECK ---

COMPUTER: OKAY

PROGRAM: OKAY

SOFTWARE DATE: 02/20/01

HEATERS

SAMPLE CHAMBER: 49c

BREATH TUBE: 40c

BAROMETER: 30.30 in

FLOW DETECTOR: OKAY

PUMP

HIGH SPEED: OKAY

DETECTOR: OKAY

FILTERS: OKAY

QUARTZ STANDARD: OKAY

CALIBRATION: OKAY

### PRINTER TEST

!"#\$%&'()\*+,-./0123456789:;<=>@ABCDEFGHIJ  
KLMNOPQRSTUVWXYZ[\]^\_`abcde fghijklmno  
pqrstuvwxyz{|}~