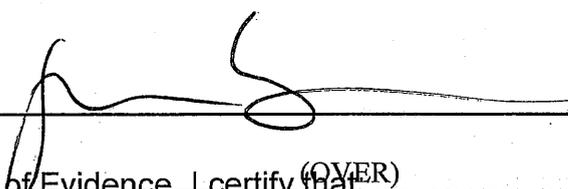


VERIFICATION OF CALIBRATION REPORT

Of Data Master cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statedwide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	130569 ✓		
Name	John Hodges	ID #	2999	Date	5/29/2008 ✓
Agency	Cordova Police Department	Phone #	424-6100		
Instrument Location	Cordova Police Department ✓				
Alco S/N	X124656 ✓	Target Value	0.076 ✓	High Pressure	900 psi
Alco Test Value Average	0.078 ✓		0.078 ✓		
	1st Alco		2nd Alco		
Signature					COB 6/13/08


Under the Alaska Rules of Evidence, I certify that, (OVER)

(a) I am Jeanne Swartz, Forensic Scientist III, Scientific Crime Detection Laboratory, State of Alaska Department of Public Safety, and was, at the time of signing, the custodian of the records of the aforementioned laboratory and the signature was made in my official capacity as Scientific Director Designee of the State Breath Alcohol Testing Program.

(b) The verification of calibration for the above instrument has been received and reviewed. Instrument operator, John Hodges, whose name appears in my records, is qualified to verify the calibration of the above instrument.

(c) This instrument is certified for evidentiary use and these records are being retained as original documents in my custody.

Signed and sealed,

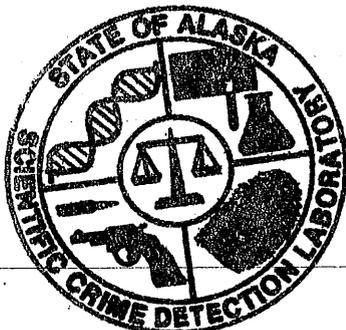



Jeanne Swartz
Scientific Director Designee
State of Alaska
State Breath Alcohol Testing Program

6/16/08

Date

VERIFICATION OF CALIBRATION REPORT

Of Data Master cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statedwide Breath Alcohol Program

DataMaster cdm S/N

130569 ✓

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130569

MAY 29, 2008

OPERATOR'S NAME:

HODGES, JOHN

OPERATOR'S NUMBER: 2999

SUBJECT'S LAST NAME:

VERIFICATION OF CAL

SUBJECT'S FIRST NAME/MI :

X

O.L. #: X

DEPT/AGENCY: CDVI

CASE/REPORT: X

TEST TYPE: V

ALCO TARGET VALUE: .076 ✓

ALCO S/N: X124656 ✓

--- BREATH ANALYSIS ---

.076 ADJUSTED FOR 30.14 in
ALCO TARGET .076 20:20
BLANK TEST .000 20:21
INTERNAL STANDARD VERIFIED 20:21
ALCO TV 30.14 in .078 ✓ 20:21
BLANK TEST .000 20:22
SUBJECT SAMPLE .000 20:23
BLANK TEST .000 20:24
ALCO TV 30.14 in .078 20:25
BLANK TEST .000 20:26

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130569

MAY 29, 2008 ✓

TIME 20:26

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY
PROGRAM: OKAY
SOFTWARE DATE: 02/20/01
HEATERS
SAMPLE CHAMBER: 49c
BREATH TUBE: 43c
BAROMETER: 30.14 in
FLOW DETECTOR: OKAY
PUMP
HIGH SPEED: OKAY
DETECTOR: OKAY
FILTERS: OKAY
QUARTZ STANDARD: OKAY
CALIBRATION: OKAY

PRINTER TEST

! " # % & ' () * + , - . / 0 1 2 3 4 5 6 7 8 9 : ; < = > ? @ A B C D E F G
H I J K L M N O P Q R S T U V W X Y Z [\] ^ _ ` a b c d e f g h i j k l m n o
p q r s t u v w x y z { | } ~