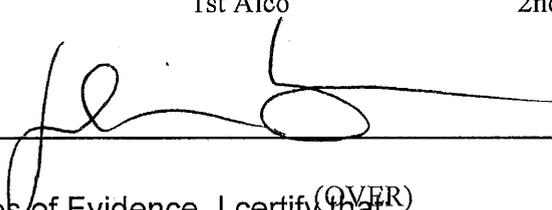


VERIFICATION OF CALIBRATION REPORT

Of Data Master cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statedwide Breath Alcohol Program


		DataMaster cdm S/N	130569
Supervisor/Operator Performing the Verification Procedure:			
A	Name	John Hodges	ID # 2999 Date 7/30/2008 ✓
	Agency	Cordova Police Department ✓	Phone # 424-6100
	Instrument Location	Cordova Police Department	
B			
	Alco S/N	X124656 ✓	Target Value 0.076 ✓ High Pressure 500psi
	Alco Test Value Average	0.078 ✓	0.078 ✓
		1st Alco	2nd Alco
	Signature		
		COB 8/12/08	

Under the Alaska Rules of Evidence, I certify that, (OVER)


(a) I am Jeanne Swartz, Forensic Scientist III, Scientific Crime Detection Laboratory, State of Alaska Department of Public Safety, and was, at the time of signing, the custodian of the records of the aforementioned laboratory and the signature was made in my official capacity as Scientific Director Designee of the State Breath Alcohol Testing Program.

(b) The verification of calibration for the above instrument has been received and reviewed. Instrument operator, John Hodges, whose name appears in my records, is qualified to verify the calibration of the above instrument.

(c) This instrument is certified for evidentiary use and these records are being retained as original documents in my custody.

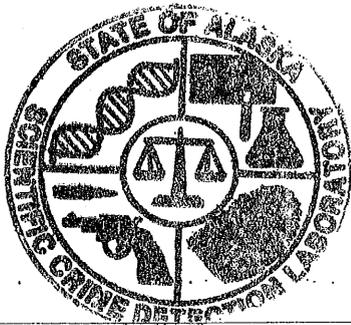

Signed and sealed,



Jeanne Swartz
Scientific Director Designee
State of Alaska
State Breath Alcohol Testing Program

8/13/08

Date

VERIFICATION OF CALIBRATION REPORT

Of Data Master cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statedwide Breath Alcohol Program

DataMaster cdm S/N

130569 ✓

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130569

JULY 30, 2000

OPERATOR'S NAME:

HODGES, JOHN

OPERATOR'S NUMBER: 2999

SUBJECT'S LAST NAME:

VERIFICATION OF CAL

SUBJECT'S FIRST NAME/MI :

X

O.L. #: X

DEPT/AGENCY: CDVI

CASE/REPORT: X

TEST TYPE: V

ALCO TARGET VALUE: .07% ✓

ALCO S/N: X124656 ✓

--- BREATH ANALYSIS ---

.07% ADJUSTED FOR 29.91 in
ALCO TARGET .075 02:50
BLANK TEST .000 02:50
INTERNAL STANDARD VERIFIED 02:51
ALCO TV 29.91 in 1.30 ✓ .07% ✓ 02:51
BLANK TEST .000 02:52
SUBJECT SAMPLE ✓ .000 ✓ 02:53
BLANK TEST .000 02:54
ALCO TV 29.91 in .07% ✓ 02:54
BLANK TEST .000 02:55

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130569

JULY 30, 2000 ✓

TIME 02:57

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY
PROGRAM: OKAY
SOFTWARE DATE: 02/20/01
HEATERS
SAMPLE CHAMBER: 49c
BREATH TUBE: 40c
BAROMETER: 29.91 in
FLOW DETECTOR: OKAY
PUMP
HIGH SPEED: OKAY
DETECTOR: OKAY
FILTERS: OKAY
QUARTZ STANDARD: OKAY
CALIBRATION: OKAY

PRINTER TEST

!@#%&'()*+,-./0123456789:;<=>?@ABCDEF6
HIJKL NOPQRSTU VWXYZ[\]^_`abcde fghijklmno
pqrstuvwxy z{|}~