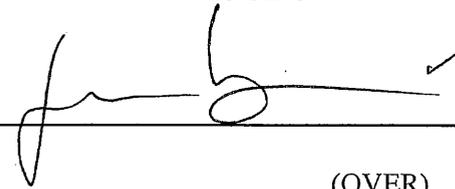


VERIFICATION OF CALIBRATION REPORT

Of Data Master cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statedwide Breath Alcohol Program

		DataMaster cdm S/N	130569 ✓
Supervisor/Operator Performing the Verification Procedure:			
Name		John Hodges	ID # 2999 Date 9/30/2008 ✓
A	Agency		Cordova Police Department Phone # 424-6100
Instrument Location		Cordova Police Department ✓	
Alco S/N		X124656 ✓	Target Value 0.076 ✓ High Pressure 500psi
B	Alco Test Value Average		0.077 ✓ 0.078 ✓
		1st Alco	2nd Alco
Signature		 ✓	
		(OVER)	

(Do Not write in the area below)

Under the Alaska Rules of Evidence, I certify that;


(a) I am Jeanne Swartz, Forensic Scientist III, Scientific Crime Detection Laboratory, State of Alaska Department of Public Safety, and was, at the time of signing, the custodian of the records of the aforementioned laboratory and the signature was made in my official capacity as Scientific Director Designee of the State Breath Alcohol Testing Program.

(b) The verification of calibration for the above instrument has been received and reviewed. Instrument operator, John Hodges, whose name appears in my records, is qualified to verify the calibration of the above instrument.

(c) This instrument is certified for evidentiary use and these records are being retained as original documents in my custody.



Signed and sealed,



Jeanne Swartz
Scientific Director Designee
State of Alaska
State Breath Alcohol Testing Program

10/24/08

Date

VERIFICATION OF CALIBRATION REPORT

Of Data Master cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statedwide Breath Alcohol Program

DataMaster cdm S/N

130569

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130569

SEPTEMBER 30, 2008

OPERATOR'S NAME:

HODGES, JOHN

OPERATOR'S NUMBER: 2999

SUBJECT'S LAST NAME:

VERIFICATION OF CAL

SUBJECT'S FIRST NAME/MI :

X

O.L. #: X

DEPT/AGENCY: CD41

CASE/REPORT: X

TEST TYPE: V

ALCO TARGET VALUE: .076

ALCO S/N: X124656

--- BREATH ANALYSIS ---

.076 ADJUSTED FOR 29.81 in
ALCO TARGET .075 16:25
BLANK TEST .000 16:26
INTERNAL STANDARD VERIFIED 16:26
ALCO TV 29.81 in .077 16:27
BLANK TEST .000 16:28
SUBJECT SAMPLE .000 16:28
BLANK TEST .000 16:29
ALCO TV 29.81 in .078 16:30
BLANK TEST .000 16:31

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130569

SEPTEMBER 30, 2008

TIME 16:40

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY

PROGRAM: OKAY

SOFTWARE DATE: 02/20/01

HEATERS

SAMPLE CHAMBER: 49c

BREATH TUBE: 41c

BAROMETER: 29.81 in

FLOW DETECTOR: OKAY

PUMP
HIGH SPEED: OKAY

DETECTOR: OKAY

FILTERS: OKAY

QUARTZ STANDARD: OKAY

CALIBRATION: OKAY

PRINTER TEST

!"#\$%&'()*+,-./0123456789:;<=>@ABCDEFGHIJKL
MNPQRSTUVWXYZ[\]^_`abcde:fghijklmnop
qrstuvwxyz{|}~