

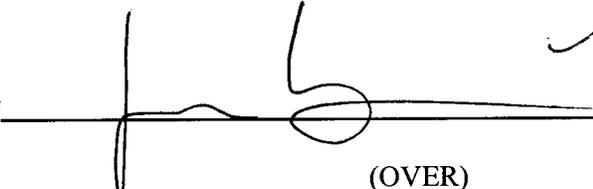
VERIFICATION OF CALIBRATION REPORT

Of Data Master cdm Breath Test Instrument

State of Alaska

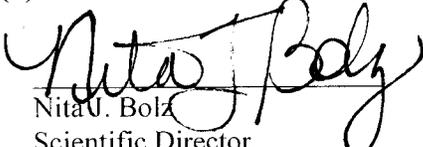
Scientific Crime Detection Laboratory - Statedwide Breath Alcohol Program

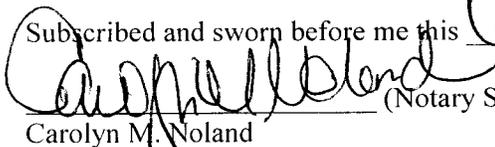
OCT 15 2009

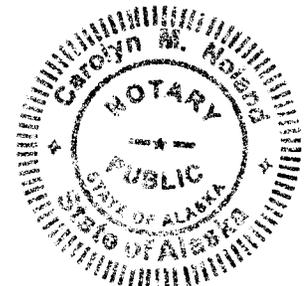
DataMaster cdm S/N <u>130569</u>	
Supervisor/Operator Performing the Verification Procedure:	
Name <u>John Hodges</u>	ID # <u>2999</u> Date <u>10/13/2009</u>
Agency <u>Cordova Police Department</u>	Phone # <u>424-6100</u>
Instrument Location <u>Cordova Police Department</u>	
Alco S/N <u>X124634</u> Target Value <u>0.078</u> High Pressure <u>250psi</u>	
Alco Test Value Average <u>0.080</u>	<u>0.080</u>
1st Alco	2nd Alco
Signature 	
(OVER) 	

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of ~~(Alaska Scientific Crime Detection Laboratory)~~ ^(Alaska Scientific Crime Detection Laboratory).
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.


Nita J. Bolz
Scientific Director
State Breath Alcohol Program

Subscribed and sworn before me this 10th day of Nov., 2009.

(Notary Seal Stamp)
Carolyn M. Noland
Notary Public, State of Alaska
Commission Expires with Office



VERIFICATION OF CALIBRATION REPORT

Of Data Master cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statedwide Breath Alcohol Program

DataMaster cdm S/N

130569

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130569

OCTOBER 13, 2009

OPERATOR'S NAME:

HODGES, JOHN

OPERATOR'S NUMBER: 8999

SUBJECT'S LAST NAME:

VERIFICATION OF CAL

SUBJECT'S FIRST NAME/MI :

X

O.L. #: X

DEPT/AGENCY: CDVI

CASE/REPORT: X

TEST TYPE: V

ALCO TARGET VALUE: .078

ALCO Q/M: K124634

--- BREATH ANALYSIS ---

.078 ADJUSTED FOR 29.83 in
ALCO TARGET .077 11:02
BLANK TEST .000 11:03
INTERNAL STANDARD VERIFIED 11:03
ALCO TV 29.83 in .000 11:03
BLANK TEST .000 11:04
SUBJECT SAMPLE .000 11:05
BLANK TEST .000 11:06
ALCO TV 29.85 in .078 11:06
BLANK TEST .000 11:07

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130569

OCTOBER 13, 2009

TIME 11:06

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY
PROGRAM: OKAY
SOFTWARE DATE: 09/08/01
VENTERS
SAMPLE CHAMBER: 48c
BREATH TUBE: 48c
BAROMETER: 29.85 in
FLOW DETECTOR: OKAY
PUMP
KOP (SET): OKAY
DETECTOR: OKAY
FILTERS: OKAY
CHECK STANDARD: OKAY
CALIBRATION: OKAY

PRINTER TEST

11/13/09 11:06:00
ALCO TARGET VALUE: .078
ALCO TV 29.85 in .078