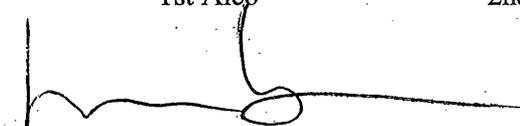


VERIFICATION OF CALIBRATION REPORT

Of Data Master cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statedwide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	130569	✓
A	Name	John Hodges	ID # 2999	Date 12/22/2008 ✓
	Agency	Cordova Police Department	Phone # 424-6100	
	Instrument Location	Cordova Police Department		✓
B	Alco S/N	X124634 ✓	Target Value 0.078 ✓	High Pressure 1100psi
	Alco Test Value Average	0.081 ✓	0.081 ✓	
		1st Alco	2nd Alco	
	Signature			CSB 1/6/09


Under the Alaska Rules of Evidence, I certify that, (OVER)


(Do Not write in the area below)
(a) I am Jeanne Swartz, Forensic Scientist III, Scientific Crime Detection Laboratory, State of Alaska Department of Public Safety, and was, at the time of signing, the custodian of the records of the aforementioned laboratory and the signature was made in my official capacity as Scientific Director Designee of the State Breath Alcohol Testing Program.

(b) The verification of calibration for the above instrument has been received and reviewed. Instrument operator, John Hodges, whose name appears in my records, is qualified to verify the calibration of the above instrument.

(c) This instrument is certified for evidentiary use and these records are being retained as original documents in my custody.

Signed and sealed,

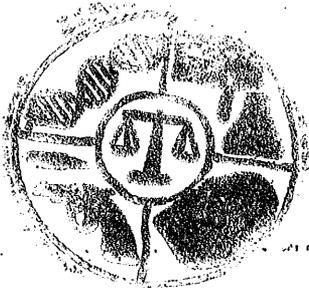



Jeanne Swartz
Scientific Director Designee
State of Alaska
State Breath Alcohol Testing Program

1/6/09
Date

VERIFICATION OF CALIBRATION REPORT

Of Data Master cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statedwide Breath Alcohol Program

DataMaster cdm S/N

130569 ✓

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130569

DECEMBER 22, 2008 ✓

OPERATOR'S NAME: ^{CB} HODGES, JOHN
OPERATOR'S NUMBER: 2999
SUBJECT'S LAST NAME: ₁₁₆₁₉
VERIFICATION OF CAL
SUBJECT'S FIRST NAME/NI :
X

O.L. #: X
DEPT/AGENCY: CDVI
CASE/REPORT: X
TEST TYPE: V
ALCO TARGET VALUE: .078 ✓
ALCO S/N: K124634

--- BREATH ANALYSIS ---

.078 ADJUSTED FOR 30.14 in		
ALCO TARGET	.078	04:05
BLANK TEST	.000	04:06
INTERNAL STANDARD	VERIFIED	04:06
ALCO TV 30.14 in	.001 ✓	04:08
BLANK TEST	.000	04:08
SUBJECT SAMPLE	.000	04:09
BLANK TEST	.000	04:10
ALCO TV 30.16 in	.001 ✓	04:11
BLANK TEST	.000	04:12

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130569

DECEMBER 22, 2008 ✓
TIME 04:16

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY

PROGRAM: OKAY

SOFTWARE DATE: 02/20/01

HEATERS

SAMPLE CHAMBER: 45c

BREATH TUBE: 41c

BAROMETER: 30.14 in

FLOW DETECTOR: OKAY

PUMP

HIGH SPEED: OKAY

DETECTOR: OKAY

FILTERS: OKAY

QUARTZ STANDARD: OKAY

CALIBRATION: OKAY

PRINTER TEST

! " # \$ % ' () * + , - . / 0 1 2 3 4 5 6 7 8 9 : ; < = > ? @ A B C D E F G
H I J K L M N O P Q R S T U V W X Y Z [\] ^ _ ` a b c d e f g h i j k l m n o
p q r s t u v w x y z { | } ~