

VERIFICATION OF CALIBRATION REPORT

Of Data Master cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statedwide Breath Alcohol Program


JUN 16 2010


Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	130569	✓			
A	Name	Mac Burrell	ID #	4756	Date	6/9/2010	✓
	Agency	Cordova Police Department	Phone #	424-6100			
	Instrument Location	Cordova Police Department					✓
	Alco S/N	X301080 X124634	Target Value	0.086	High Pressure	600	✓
B	Alco Test Value Average	0.087	1st Alco	0.087	2nd Alco		✓
	Signature	Mac Burrell					✓
							COB 6/18/10

(OVER)



I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (Do Not write in the area below)
- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
 - (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
 - (3) I am the Scientific Director of the State Breath Alcohol Program.
 - (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
 - (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
 - (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

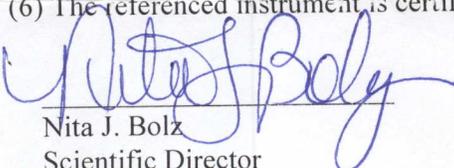
Nita J. Bolz
Scientific Director
State Breath Alcohol Program

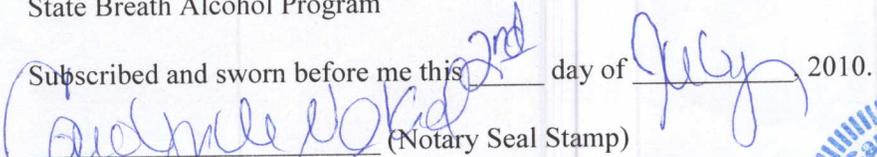Subscribed and sworn before me this 2nd day of July, 2010.


Carolyn M. Noland
Notary Public, State of Alaska
Commission Expires with Office

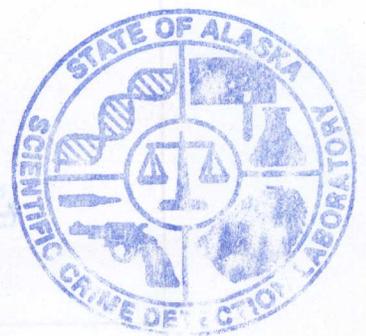

VERIFICATION OF CALIBRATION REPORT

Of Data Master cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statedwide Breath Alcohol Program

DataMaster cdm S/N

130569 ✓

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130569 ✓

JUNE 09, 2010 ✓

OPERATOR'S NAME:

DURRELL/M

OPERATOR'S NUMBER: 4756

SUBJECT'S LAST NAME:

VERIFICATION OF CAL

SUBJECT'S FIRST NAME/MI :

X

O.L. #: X

DEPT/AGENCY: CDVI

CASE/REPORT: 060910

TEST TYPE: V

ALCO TARGET VALUE: .006 ✓

ALCO S/N: K301636 ✓

--- BREATH ANALYSIS ---

.006 ADJUSTED FOR 30.17 in

ALCO TARGET	.006	12:00
BLANK TEST	.000	12:01
INTERNAL STANDARD	VERIFIED	12:01
ALCO TV 30.17 in	.007 ✓	12:01
BLANK TEST	.000	12:02
SUBJECT SAMPLE	.000	12:03
BLANK TEST	.000	12:04
ALCO TV 30.19 in	.007 ✓	12:05
BLANK TEST	.000	12:05

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130569 ✓

JUNE 09, 2010 ✓
TIME 11:45

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY
PROGRAM: OKAY
SOFTWARE DATE: 02/20/01
HEATERS
SAMPLE CHAMBER: 43c
BREATH TUBE: 43c
BAROMETER: 30.17 in
FLOW DETECTOR: OKAY
PUMP
HIGH SPEED: OKAY
DETECTOR: OKAY
FILTERS: OKAY
QUARTZ STANDARD: OKAY
CALIBRATION: OKAY

PRINTER TEST

!##\$%&'()*+,-./0123456789:;<=>@ABCDEFGHIJKL
HIJKLMNOPQRSTUVWXYZ[\]^_`abcde fghijklmnop
qrstuvwxyz{|}~?@