

JAN 19 2011 <sup>2011</sup> <sub>2010</sub> <sup>an</sup> <sub>3/1/11</sub>

**VERIFICATION OF CALIBRATION REPORT**  
*of DataMaster cdm Breath Test Instrument*  
*State of Alaska*  
*Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program*

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	<u>130570</u> ✓
Name	<u>STEVE DUNN</u>	ID#	<u>4106</u> ✓
		Date	<u>1-14-11</u> ✓
A	Agency	<u>APD</u>	Phone # <u>786-8900</u>
	Instrument Location	<u>4<sup>th</sup> AVE SUB</u>	
B	Alco S/N	<u>X124611</u> ✓	Target Value <u>.081</u> ✓
		High Pressure	<u>650 PSF</u>
	Alco Test Values	<u>.081</u> ✓ 1 <sup>st</sup> Alco	<u>.081</u> ✓ 2 <sup>nd</sup> Alco
	Signature		


(OVER)

*amb*  
*2/8/11*

(Do Not write in the area below)

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:


- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

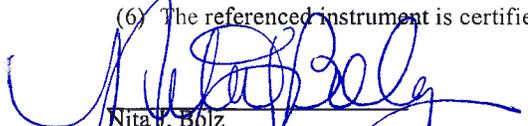  
Nita J. Bolz  
Scientific Director  
State Breath Alcohol Program

Subscribed and sworn before me this 11<sup>th</sup> day of MAR, 2011 <sup>an</sup> <sub>2010</sub>

 (Notary Seal Stamp)

Daniel L. Nicholas  
Notary Public, State of Alaska  
Commission Expires with Office

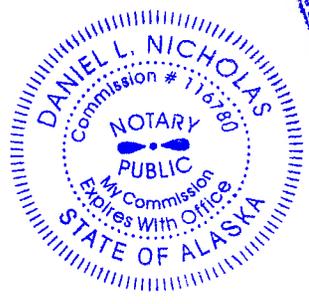

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N **130570**

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

*S. DUNN  
\* 1361*

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130570

JANUARY 14, 2011

OPERATOR'S NAME:

DUNN/S

OPERATOR'S NUMBER: 4106

SUBJECT'S LAST NAME:

VERIFICATION OF CAL

SUBJECT'S FIRST NAME/NI :

V

O.L. #: V

DEPT/AGENCY: ANCI

CASE/REPORT: V

TEST TYPE: V

ALCO TARGET VALUE: .001

ALCO S/N: X124611

### --- BREATH ANALYSIS ---

.001 ADJUSTED FOR 30.22 in  
ALCO TARGET .001 11:54  
BLANK TEST .000 11:55  
INTERNAL STANDARD VERIFIED 11:55  
ALCO TV 30.22 in .001 11:56  
BLANK TEST .000 11:56  
SUBJECT SAMPLE .000 11:57  
BLANK TEST .000 11:58  
ALCO TV 30.22 in .001 11:58  
BLANK TEST .000 11:59

*S. DUNN  
\* 1361*

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130570

JANUARY 14, 2011

TIME 11:51

### --- DIAGNOSTIC CHECK ---

COMPUTER: OKAY  
PROGRAM: OKAY  
SOFTWARE DATE: 12/11/00  
HEATERS  
SAMPLE CHAMBER: 50c  
BREATH TUBE: 42c  
BAROMETER: 30.22 in  
FLOW DETECTOR: OKAY  
PUMP  
HIGH SPEED: OKAY  
DETECTOR: OKAY  
FILTERS: OKAY  
QUARTZ STANDARD: OKAY  
CALIBRATION: OKAY

### PRINTER TEST

!"#\$%&'()\*+,-./0123456789:;<=>?@ABCDEFGHIJKL  
MNOPQRSTUVWXYZ[\]^\_`abcdefghijklmnop  
qrstuvwxyz{|}~