

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program


Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N <u>130570</u> ✓
Name <u>APD STEVE DUNN</u> ID# <u>4106</u> Date <u>8-22-08</u> ✓		
A	Agency <u>APD</u> Phone # _____	
	Instrument Location <u>42 AVE SUB.</u> ✓	
Alco S/N <u>58428</u> ✓ Target Value <u>.078</u> ✓ High Pressure <u>1300</u> ✓		
B	Alco Test Value Average <u>.079</u> ✓ <u>.078</u> ✓	
	1 st Alco 2 nd Alco	
Signature <u>[Signature]</u> ✓		<u>CSB</u> <u>12/5/08</u>
(OVER)		

Under the Alaska Rules of Evidence, I certify that:
(Do Not write in the area below)

(a) I am Jeanne Swartz, Forensic Scientist III, Scientific Crime Detection Laboratory, State of Alaska Department of Public Safety, and was, at the time of signing, the custodian of the records of the aforementioned laboratory and the signature was made in my official capacity as Scientific Director Designee of the State Breath Alcohol Testing Program.

(b) The verification of calibration for the above instrument has been received and reviewed. Instrument operator, Steve P Dunn, whose name appears in my records, is qualified to verify the calibration of the above instrument.

(c) This instrument is certified for evidentiary use and these records are being retained as original documents in my custody.

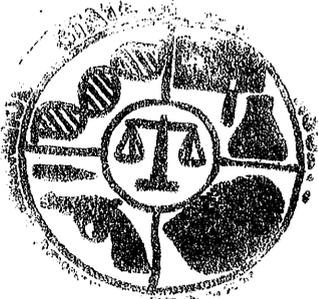

Signed and sealed,

[Signature]

Jeanne Swartz
Scientific Director Designee
State of Alaska
State Breath Alcohol Testing Program

12/5/08
Date

DEC 04 2008

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130570 ✓

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

S. DUNN #1361

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130570

AUGUST 22, 2008 ✓ *CSB 12/5/08*

OPERATOR'S NAME:

DUNN/S

OPERATOR'S NUMBER: 4106

SUBJECT'S LAST NAME:

VERIFICATION OF CAL

SUBJECT'S FIRST NAME/MI:

V

O.L. #: V

DEPT/AGENCY: ANCI

CASE/REPORT: V

TEST TYPE: V

ALCO TARGET VALUE: .078 ✓

ALCO S/N: 58428

--- BREATH ANALYSIS ---

.078 ADJUSTED FOR 29.67 in
ALCO TARGET .077 19:22
BLANK TEST .000 19:23
INTERNAL STANDARD VERIFIED 19:23
ALCO TV 29.67 in .079 ✓ 19:23
BLANK TEST .000 19:24
SUBJECT SAMPLE *CSB 12/5/08* .000 19:25
BLANK TEST .000 19:25
ALCO TV 29.67 in .078 ✓ 19:26
BLANK TEST .000 19:27

DIAGNOSTIC CHECK

S. DUNN #1361

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130570

AUGUST 22, 2008 ✓
TIME 19:20

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY
PROGRAM: OKAY
SOFTWARE DATE: 02/20/01
HEATERS
SAMPLE CHAMBER: 50c
BREATH TUBE: 40c
BAROMETER: 29.68 in
FLOW DETECTOR: OKAY
PUMP
HIGH SPEED: OKAY
DETECTOR: OKAY
FILTERS: OKAY
QUARTZ STANDARD: OKAY
CALIBRATION: OKAY

PRINTER TEST

!"#\$%&'()*+,-./0123456789:;<=>?@ABCDEFGHIJKL
MNPQRSTUVWXYZ[\]^_`abcdefghijklmnopqr
stuvwxyz{|}~