

# VERIFICATION OF CALIBRATION REPORT

*of DataMaster cdm Breath Test Instrument  
State of Alaska*

*Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program*

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	<u>130570</u> ✓
Name	<u>C. RITAK</u>	ID#	<u>3791</u> ✓
		Date	<u>10/1/10</u> ✓
A	Agency	<u>APD</u>	Phone # <u>786-2640</u>
	Instrument Location	<u>4th AVE SUB STATION</u>	
B	Alco S/N	<u>X124611</u> ✓	Target Value <u>-0.081</u> ✓
		High Pressure	<u>1100</u>
	Alco Test Values	<u>0.77</u> ✓ 1st Alco	<u>0.77</u> ✓ 2nd Alco
	Signature	<u>[Signature]</u> RITAK/1349	

(OVER)

BMB  
10/5/10

(Do Not write in the area below)


I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

[Signature]  
Nita J. Bolz  
Scientific Director  
State Breath Alcohol Program

Subscribed and sworn before me this 16th day of DEC, 2010.

[Signature] (Notary Seal Stamp)  
Daniel L. Nicholas  
Notary Public, State of Alaska  
Commission Expires with Office

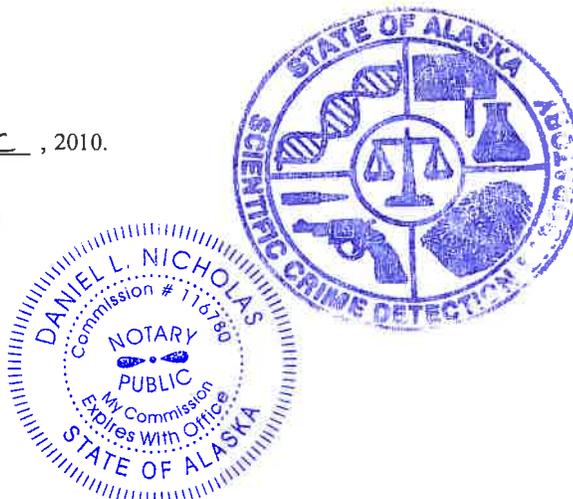

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument  
State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N

130570

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130570

OCTOBER 01, 2010

OPERATOR'S NAME:  
RITALA

OPERATOR'S NUMBER: 3791

SUBJECT'S LAST NAME:

VERIFICATION OF CALIBRATION

SUBJECT'S FIRST NAME/MI :

NEW ALCO

O.L. #: A

DEPT/AGENCY: ANCI

CASE/REPORT: A

TEST TYPE: V

ALCO TARGET VALUE: 001

ALCO S/N: X124611

--- BREATH ANALYSIS ---

.001 ADJUSTED FOR 29.18 in  
ALCO TARGET .079 18:24  
BLANK TEST .000 18:25  
INTERNAL STANDARD VERIFIED 18:25  
ALCO TV 29.18 in .077 18:25  
BLANK TEST .000 18:26  
SUBJECT SAMPLE .000 18:26  
BLANK TEST .000 18:27  
ALCO TV 29.18 in .077 18:27  
BLANK TEST .000 18:28

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130570

OCTOBER 01, 2010  
TIME 18:17

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY  
PROGRAM: OKAY  
SOFTWARE DATE: 12/11/98  
HEATERS  
SAMPLE CHAMBER: 52c  
BREATH TUBE: 41c  
BAROMETER: 29.16 in  
FLOW DETECTOR: OKAY  
PUMP  
HIGH SPEED: OKAY  
DETECTOR: OKAY  
FILTERS: OKAY  
QUARTZ STANDARD: OKAY  
CALIBRATION: OKAY

F-PRINTER TEST

!"#\$%&'()\*+,-./0123456789:;<=>?@ABCDEF6  
HIJKLHNDOPQRSTUWVXYZ[\]^\_`abcde+ghijklmno  
pqrstuvwxyz{|}~`