

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

12/18/09

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program


Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	130570
Name	C. RITALA	ID#	3791
		Date	11/18/09
A	Agency	APD	Phone # 786 2640
	Instrument Location	FLORA SUB STATION (4th AVE)	
B	Alco S/N	X124669	Target Value
			0.081 ✓
			0.076
		High Pressure	1100
	Alco Test Value Average	-081 ✓	082 ✓
		1 st Alco	2 nd Alco
	Signature		RITALA/1349
			 12/14/09

(OVER)

(Do Not write in the area below)


I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

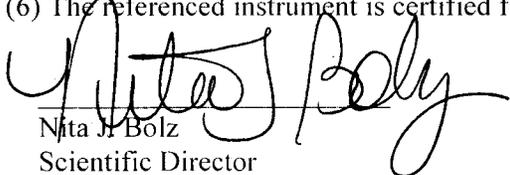

Nita J. Bolz
Scientific Director
State Breath Alcohol Program

Subscribed and sworn before me this 25th day of January 2010

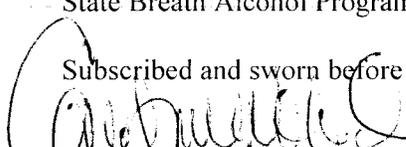 (Notary Seal Stamp)

Carolyn M. Noland
Notary Public, State of Alaska
Commission Expires with Office

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130570 ✓

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130570

NOVEMBER 10, 2009

OPERATOR'S NAME:

RITALA

OPERATOR'S NUMBER: 3791

SUBJECT'S LAST NAME:

VERIFICATION OF CALIBRATION

SUBJECT'S FIRST NAME/MI :

INSTALL NEW ALCO

O.L. #: A

DEPT/AGENCY: ANCI

CASE/REPORT: A

TEST TYPE: V

ALCO TARGET VALUE: 0.084 ✓

ALCO S/N: X124659 ✓

--- BREATH ANALYSIS ---

.076 ADJUSTED FOR 29.91 in ✓

ALCO TARGET .075 22:52

BLANK TEST .000 22:53

INTERNAL STANDARD VERIFIED 22:53

ALCO TV 29.91 in .001 22:53

BLANK TEST .000 22:54

SUBJECT SAMPLE 0.084 22:55

BLANK TEST .000 22:55

ALCO TV 29.91 in .002 22:56

BLANK TEST .000 22:56

CR 1349 11/10/09

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130570

NOVEMBER 10, 2009 ✓

TIME 22:49

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY

PROGRAM: OKAY

SOFTWARE DATE: 12/11/08

HEATERS

SAMPLE CHAMBER: 50c

BREATH TUBE: 42c

BAROMETER: 29.91 in

FLOW DETECTOR: OKAY

PUMP

HIGH SPEED: OKAY

DETECTOR: OKAY

FILTERS: OKAY

QUARTZ STANDARD: OKAY

CALIBRATION: OKAY

PRINTER TEST

!##%&'()*+,-./0123456789:;<=^_`{|}~@ABCDEFGHI
HIJKLMNOPQRSTUVWXYZ[\]^_`{|}~@ABCDEFGHI
pqrstuvwxyz{|}~@

CR 1349 11/10/09

Target value changed at 5:00 PM (0.084) COS 12/23/09
recalculated NTS 11/21/10
COS 12/23/09