

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program


DataMaster cdm S/N <u>130570</u>	
Supervisor/Operator Performing the Verification Procedure:	
Name <u>STEVE DUNN</u>	ID# <u>4106</u> Date <u>3-18-11</u>
A Agency <u>APD</u>	Phone # <u>786-8900</u>
Instrument Location <u>4th AVE SUB.</u>	
B Alco S/N <u>X124611</u> Target Value <u>.081</u> High Pressure <u>600 PSI</u>	
Alco Test Values <u>.081</u> <u>.082</u>	
1 st Alco 2 nd Alco	
Signature 	
(OVER)	

Handwritten initials and date:
SMB
3/18/11

(Do Not write in the area below)


I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

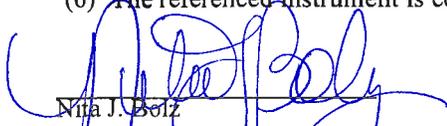
Nita J. Bolz
Scientific Director
State Breath Alcohol Program

Subscribed and sworn before me this 1ST day of APRIL, 2011 AN


(Notary Seal Stamp)
Daniel L. Nicholas
Notary Public, State of Alaska
Commission Expires with Office

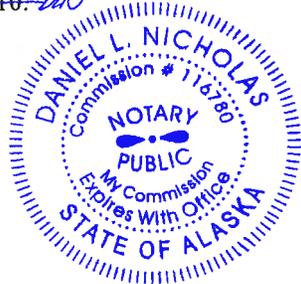

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N

130570

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

S. DUNN #1361

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130570

MARCH 18, 2011

OPERATOR'S NAME: *AMB 3/31/11*
DUNN/S
OPERATOR'S NUMBER: 4106
SUBJECT'S LAST NAME:
VERIFICATION OF CAL
SUBJECT'S FIRST NAME/MI :
V

O.L. #: V
DEPT/AGENCY: ANCI
CASE/REPORT: V
TEST TYPE: V
ALCO TARGET VALUE: .081
ALCO S/N: X124611

--- BREATH ANALYSIS ---

.081 ADJUSTED FOR 30.25 in		
ALCO TARGET	.081	10:15
BLANK TEST	.000	10:16
INTERNAL STANDARD	VERIFIED	10:16
ALCO TV 30.25 in	.081	10:17
BLANK TEST	.000	10:17
SUBJECT SAMPLE <i>AMB 3/31/11</i>	.200	10:19
BLANK TEST	.000	10:19
ALCO TV 30.25 in	.082	10:20
BLANK TEST	.000	10:20

DIAGNOSTIC CHECK

S. DUNN #1361

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130570

MARCH 18, 2011
TIME 10:18

--- DIAGNOSTIC CHECK ---

COMPUTER:	OKAY
PROGRAM:	OKAY
SOFTWARE DATE:	12/11/08
HEATERS	
SAMPLE CHAMBER:	50c
BREATH TUBE:	41c
BAROMETER:	30.25 in
FLOW DETECTOR:	OKAY
PUMP	
HIGH SPEED:	OKAY
DETECTOR:	OKAY
FILTERS:	OKAY
QUARTZ STANDARD:	OKAY
CALIBRATION:	OKAY

PRINTER TEST

!"#\$%&'()*+,-./0123456789:;<=>?@ABCDEFGHIJKL
MNPQRSTUVWXYZ[\]^_`abcdefgijklmnop
qrstuvwxyz{|}~