

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

FEB 12 2009


Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	<u>130571</u> ✓
Name		<u>C. RITALA</u>	ID# <u>3791</u> Date <u>2/10/09</u> ✓
A	Agency	<u>APD</u>	Phone # <u>786-2640</u>
Instrument Location		<u>ANCHORAGE JAIL</u> ✓	
Alco S/N		<u>X172946</u> ✓	Target Value <u>.082</u> ✓ High Pressure <u>900</u>
B	Alco Test Value Average		<u>.080</u> ✓ <u>.081</u> ✓
		1 st Alco	2 nd Alco
Signature		<u>Chris Ritala</u> ✓	<u>CRS</u> <u>2/23/09</u>
(OVER)			

Under the Alaska Rules of Evidence, I certify that, (Do Not write in the area below)

(a) I am Jeanne Swartz, Forensic Scientist III, Scientific Crime Detection Laboratory, State of Alaska Department of Public Safety, and was, at the time of signing, the custodian of the records of the aforementioned laboratory and the signature was made in my official capacity as Scientific Director Designee of the State Breath Alcohol Testing Program.

(b) The verification of calibration for the above instrument has been received and reviewed. Instrument operator, Chris Ritala, whose name appears in my records, is qualified to verify the calibration of the above instrument.

(c) This instrument is certified for evidentiary use and these records are being retained as original documents in my custody.

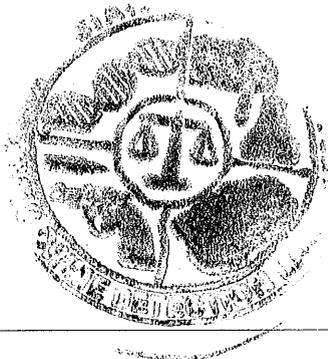

Signed and sealed

Jeanne Swartz

Jeanne Swartz
Scientific Director Designee
State of Alaska
State Breath Alcohol Testing Program

02/23/09

Date

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130571 ✓

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130571

FEBRUARY 10, 2009 ✓ *2/13/09*

OPERATOR'S NAME:

RITALA

OPERATOR'S NUMBER: 3791

SUBJECT'S LAST NAME:

VERIFICATION OF CALIBRATION

SUBJECT'S FIRST NAME/MI :

A

O.L. #: A

DEPT/AGENCY: ANCI

CASE/REPORT: A

TEST TYPE: V

ALCO TARGET VALUE: .002 ✓ *2/10/09*

ALCO S/N: X172946

--- BREATH ANALYSIS ---

0.002
.002 ADJUSTED FOR 30.14 in
ALCO TARGET .002 19:19
BLANK TEST .000 19:19
INTERNAL STANDARD VERIFIED 19:20
ALCO TV 30.14 in .000 ✓ 19:20
BLANK TEST .000 19:21
SUBJECT SAMPLE *0.002* ✓ 19:22
BLANK TEST .000 19:23
ALCO TV 30.14 in .001 ✓ 19:23
BLANK TEST .000 19:24

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130571

FEBRUARY 10, 2009 ✓
TIME 19:15

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY

PROGRAM: OKAY

SOFTWARE DATE: 12/11/08

HEATERS

SAMPLE CHAMBER: 50c

BREATH TUBE: 42c

BAROMETER: 30.14 in

FLOW DETECTOR: OKAY

PUMP

HIGH SPEED: OKAY

DETECTOR: OKAY *2/13/09*

FILTERS: OKAY *2/10/09*

QUARTZ STANDARD: OKAY

CALIBRATION: OKAY

PRINTER TEST

!"#\$%&'()*+,-./0123456789:;<=>@ABCDEFGHIJKL
MNPQRSTUVWXYZ[\]^_`abcdefghijklmnopqr
stuvwxyz{|}~*