

VERIFICATION OF CALIBRATION REPORT MAY 17 2010
of DataMaster edm Breath Test Instrument
State of Alaska
Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor Operator Performing the Verification Procedure:		DataMaster edm S/N	130571
Name	JEFFREY L EUBIE	ID#	6623 Date 4-29-10
Agency	Anchorage Police Dept	Phone #	786-8900
Instrument Location	Secly Substation		
Alco S/N		X172931	Target Value .082 High Pressure 250
Alco Test Values		.085	.084
		1 st Alco	2 nd Alco
Signature			

(OVER)


(Do Not write in the area below)


AMB
5/24/10

- I, Nita J. Bolz, after being first duly sworn, depose and state as follows:
- I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
 - The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
 - I am the Scientific Director of the State Breath Alcohol Program.
 - In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
 - The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
 - The referenced instrument is certified for evidentiary use in the State of Alaska.


 Nita J. Bolz
 Scientific Director
 State Breath Alcohol Program

Subscribed and sworn before me this 24th day of JUNE, 2010.

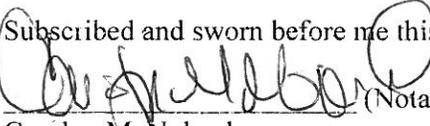
 Carolyn M. Noland
 Notary Public, State of Alaska
 Commission Expires with Office

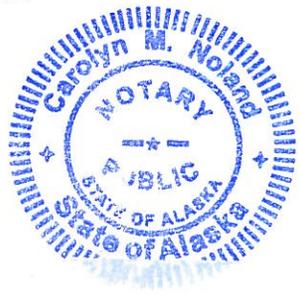

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130571

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130571

APRIL 29, 2010

OPERATOR'S NAME:

ELBIE/JEFFREY/L

OPERATOR'S NUMBER: 6623

SUBJECT'S LAST NAME:

TEST-VOC

SUBJECT'S FIRST NAME/MI :

TEST-VOC

O.L. #: 00000

DEPT/AGENCY: ANCI

CASE/REPORT: 10-000

TEST TYPE: V

ALCO TARGET VALUE: .082

ALCO S/N: X172931

--- BREATH ANALYSIS ---

.082 ADJUSTED FOR 30.09 in

ALCO TARGET	.082	23:47
BLANK TEST	.000	23:48
INTERNAL STANDARD	VERIFIED	23:48
ALCO TV 30.07 in	.085	23:48
BLANK TEST	.000	23:49
SUBJECT SAMPLE	.000	23:49
BLANK TEST	.000	23:50
ALCO TV 30.07 in	.084	23:50
BLANK TEST	.000	23:51

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130571

APRIL 29, 2010

TIME 23:38

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY

PROGRAM: OKAY

SOFTWARE DATE: 12/11/08

HEATERS

SAMPLE CHAMBER: 50c

BREATH TUBE: 41c

BAROMETER: 30.09 in

FLOW DETECTOR: OKAY

PUMP

HIGH SPEED: OKAY

DETECTOR: OKAY

FILTERS: OKAY

QUARTZ STANDARD: OKAY

CALIBRATION: OKAY

PRINTER TEST

!"#\$%&'()*+,-./0123456789:;<=>?@ABCDEF
HIJKLMN0PQRSTUWXYZ[\]^_`abcde+ghijklmno
pqrstuvwxyz{|}~"