

NOV 23 2007

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program


Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	130571
Name	Gary Yamamoto	ID#	2765
Date	11-8-07		
A Agency		Fairbanks Police Department	Phone # 459-6500
Instrument Location 911 Cushman Street Fairbanks, Alaska 99701			
B Alco S/N		78890	Target Value .078
			High Pressure 1000
Alco Test Value Average		.075	.076
		1 st Alco	2 nd Alco
Signature		<i>[Handwritten Signature]</i>	CAB 11/20/07

(OVER)

Under the Alaska Rules of Evidence, I certify that (Do not write in the area below)

- (a) I am Jeanne Swartz, Criminalist III, Scientific Crime Detection Laboratory, State of Alaska Department of Public Safety, and was, at the time of signing, the custodian of the records of the aforementioned laboratory and the signature was made in my official capacity as Scientific Director Designee of the State Breath Alcohol Testing Program.
- (b) The verification of calibration for the above instrument has been received and reviewed. Instrument operator, Gary Yamamoto, whose name appears in my records, is qualified to verify the calibration of the above instrument.
- (c) This instrument is certified for evidentiary use and these records are being retained as original documents in my custody.

Signed and sealed,

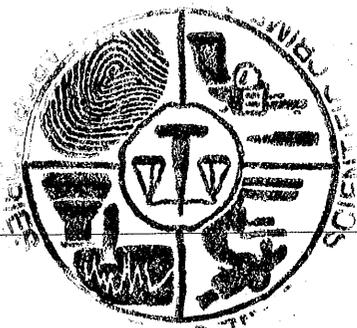

[Handwritten Signature] _____ 11/26/07
 Date
 Jeanne Swartz
 Scientific Director Designee
 State of Alaska
 State Breath Alcohol Testing Program