

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument
State of Alaska

FEB 23 2010

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor Operator Performing the Verification Procedure:		DataMaster cdm S/N	130579 ✓
Name	Noll	ID#	6520
		Date	2-15-10 ✓
Agency	APD	Phone #	746-8968
Instrument Location	Anchorage Jail South Room		
Alco S/N	630459 ✓	Target Value	1.086 ✓
		High Pressure	500
Alco Test Values	1.086 ✓	1 st Alco	1.088 ✓
		2 nd Alco	
Signature			


(OVER)

AMB
2/23/2010


(Do Not write in the area below)

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

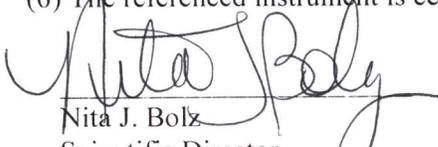
Nita J. Bolz
Scientific Director
State Breath Alcohol Program

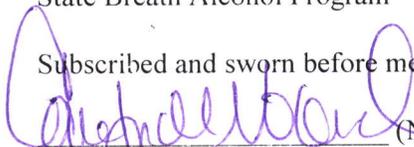

Subscribed and sworn before me this 24th day of February, 2010.
 (Notary Seal Stamp)

Carolyn M. Noland
Notary Public, State of Alaska
Commission Expires with Office



VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N

130579

2/22/10
CW

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130579

FEBRUARY 15, 2010

OPERATOR'S NAME:

NOLL

OPERATOR'S NUMBER: 6520

SUBJECT'S LAST NAME:

CALIBRATION

SUBJECT'S FIRST NAME/MI :

VERIFICATION/O

O.L. #: 012345

DEPT/AGENCY: ANCL

CASE/REPORT: 10-98765

TEST TYPE: V

ALCO TARGET VALUE: .086

ALCO S/N: G30459

--- BREATH ANALYSIS ---

.086 ADJUSTED FOR 29.75 in

ALCO TARGET	.085
BLANK TEST	.000
INTERNAL STANDARD	VERIFIED
ALCO TV 29.77 in	.088
BLANK TEST	.000
SUBJECT SAMPLE	.000
BLANK TEST	.000
ALCO TV 29.77 in	.088
BLANK TEST	.000

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130579

FEBRUARY 15, 2010

TIME 23:45

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY

PROGRAM: OKAY

SOFTWARE DATE: 12/11/08

HEATERS

SAMPLE CHAMBER: 49c

BREATH TUBE: 42c

BAROMETER: 29.77 in

FLOW DETECTOR: OKAY

PUMP

23:57 HIGH SPEED: OKAY

23:59 DETECTOR: OKAY

23:59 FILTERS: OKAY

00:00 QUARTZ STANDARD: OKAY

00:01 CALIBRATION: OKAY

00:02

00:03

00:03

PRINTER TEST

!"#\$%&'()*+,-./0123456789:;<=>?@ABCDEFGH
IJKLMNOPQRSTUVWXYZ[\]^_`abcdefghijklmnop
qrstuvwxyz{|}~^