

MAR 27 2008

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

|                                                            |        |                           |                                                   |
|------------------------------------------------------------|--------|---------------------------|---------------------------------------------------|
| Supervisor/Operator Performing the Verification Procedure: |        | DataMaster cdm S/N        | <u>130579</u>                                     |
| Name                                                       |        | <u>C. RITALA</u>          | ID# <u>3791</u> Date <u>3/26/08</u>               |
| A                                                          | Agency | <u>A.P.D</u>              | Phone # <u>796.2640</u>                           |
| Instrument Location <u>ANCHORAGE JAIL</u>                  |        |                           |                                                   |
| Alco S/N                                                   |        | <u>X301737</u>            | Target Value <u>078</u> High Pressure <u>1300</u> |
| Alco Test Value Average                                    |        | <u>079</u>                | <u>080</u>                                        |
|                                                            |        | 1 <sup>st</sup> Alco      | 2 <sup>nd</sup> Alco                              |
| Signature                                                  |        | <u>Chris Ritala</u> /1349 | <u>CRB</u><br><u>4/8/08</u>                       |


(OVER)

Under the Alaska Rules of Evidence, I certify that (If not, write in the area below)

(a) I am Jeanne Swartz, Forensic Scientist III, Scientific Crime Detection Laboratory, State of Alaska Department of Public Safety, and was, at the time of signing, the custodian of the records of the aforementioned laboratory and the signature was made in my official capacity as Scientific Director Designee of the State Breath Alcohol Testing Program.

(b) The verification of calibration for the above instrument has been received and reviewed. Instrument operator, Chris Ritala, whose name appears in my records, is qualified to verify the calibration of the above instrument.

(c) This instrument is certified for evidentiary use and these records are being retained as original documents in my custody.

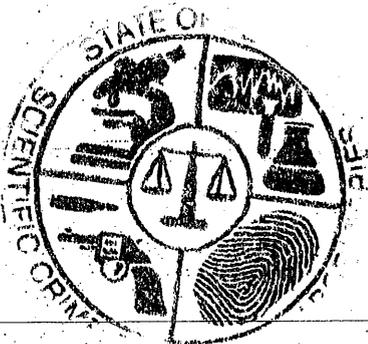

Signed and sealed,

Jeanne Swartz

Jeanne Swartz  
Scientific Director Designee  
State of Alaska  
State Breath Alcohol Testing Program

4/12/08  
Date

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130579

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130579

MARCH 26, 2008

OPERATOR'S NAME:

RITALA

OPERATOR'S NUMBER: 3791

SUBJECT'S LAST NAME:

VERIFICATION OF CALIBRATION

SUBJECT'S FIRST NAME/MI :

Z

O.L. #: Z

DEPT/AGENCY: ANCI

CASE/REPORT: A

TEST TYPE: V

ALCO TARGET VALUE: .078

ALCO S/N: X301737

--- BREATH ANALYSIS ---

.078 ADJUSTED FOR 30.07 in  
ALCO TARGET .078 20:00  
BLANK TEST .000 20:02  
INTERNAL STANDARD VERIFIED 20:02  
ALCO TV 30.07 in .079 20:02  
BLANK TEST .000 20:03  
SUBJECT SAMPLE .000 20:04  
BLANK TEST .000 20:05  
ALCO TV 30.09 in .000 20:05  
BLANK TEST .000 20:06

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130579

MARCH 26, 2008

TIME 19:57

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY

PROGRAM: OKAY

SOFTWARE DATE: 02/20/01

HEATERS

SAMPLE CHAMBER: 49c

BREATH TUBE: 41c

BAROMETER: 30.07 in

FLOW DETECTOR: OKAY

PUMP

HIGH SPEED: OKAY

DETECTOR: OKAY

FILTERS: OKAY

QUARTZ STANDARD: OKAY

CALIBRATION: OKAY

PRINTER TEST

!"#\$%&'()\*+,-./0123456789:;<=>?@ABCDEFGHIJ  
KLMNOPQRSTUVWXYZ[\]^\_`abcde fghijklmno  
pqrstuvwxyz{|}~