

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument  
State of Alaska

APR 09 2009

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure:	
Name <u>C. RITALA</u>	DataMaster cdm S/N <u>130579</u>
Agency <u>ARD</u>	ID# <u>3791</u> Date <u>4/5/09</u>
Instrument Location <u>ANCHORAGE JAIL</u>	Phone # <u>786-2640</u>
Alco S/N <u>X124630</u> Target Value <u>-084</u> High Pressure <u>500</u>	
Alco Test Value Average <u>-084</u> <u>-084</u>	
1 <sup>st</sup> Alco 2 <sup>nd</sup> Alco	
Signature <u>C. Ritala</u> <u>RITALA/1349</u>	


(OVER) CRB  
5/1/09

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.

Nita J. Bolz  
Nita J. Bolz  
Scientific Director  
State Breath Alcohol Program

Subscribed and sworn before me this 5 day of May 2009.  
Carolyn M. Noland (Notary Seal Stamp)  
Carolyn M. Noland  
Notary Public, State of Alaska  
Commission Expires with Office

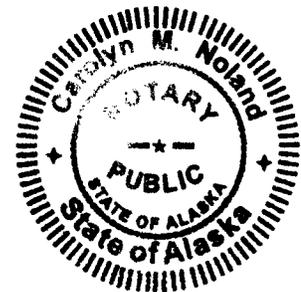

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130579

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130579

APRIL 05, 2009

OPERATOR'S NAME: RITALA  
OPERATOR'S NUMBER: 3791  
SUBJECT'S LAST NAME:  
VERIFICATION OF CALIBRATION  
SUBJECT'S FIRST NAME/MI : A

O.L. #: A  
DEPT/AGENCY: ANCI  
CASE/REPORT: A  
TEST TYPE: V  
ALCO TARGET VALUE: .084  
ALCO S/N: X124630

--- BREATH ANALYSIS ---

.084 ADJUSTED FOR 30.14 in		
ALCO TARGET	.084	03:10
BLANK TEST	.000	03:12
INTERNAL STANDARD	VERIFIED	03:12
ALCO TV 30.16 in	.084	03:12
BLANK TEST	.000	03:13
SUBJECT SAMPLE	.000	03:13
BLANK TEST	.000	03:14
ALCO TV 30.16 in	.084	03:14
BLANK TEST	.000	03:15

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130579

APRIL 05, 2009  
TIME 03:09

--- DIAGNOSTIC CHECK ---

COMPUTER:	OKAY
PROGRAM:	OKAY
SOFTWARE DATE:	12/11/08
HEATERS	
SAMPLE CHAMBER:	50c
BREATH TUBE:	42c
BAROMETER:	30.14 in
FLOW DETECTOR:	OKAY
PUMP	
HIGH SPEED:	OKAY
DETECTOR:	OKAY
FILTERS:	OKAY
QUARTZ STANDARD:	OKAY
CALIBRATION:	OKAY

PRINTER TEST  
!"#\$%&'()\*+,-./0123456789:;<=>?@ABCDEFGHIJKL  
MNOPQRSTUVWXYZ[\]^\_`abcdefgijklmno  
pqrstuvwxyz{|}~`