

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument
State of Alaska

APR 08 2010

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	130579			
Name	C. RITAK	ID#	3791			
		Date	4/6/10			
A Agency	ADP	Phone #	786-2640			
Instrument Location	ANCH JAIL					
Alco S/N		719493	Target Value	082	High Pressure	250
B Alco Test Values		081	082			
		1 st Alco	2 nd Alco			
Signature		C. RITAK				

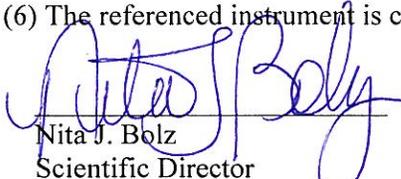
(OVER)

(Do Not write in the area below)

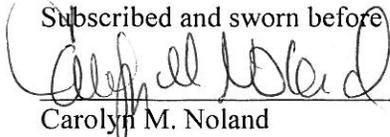
8MB
4/14/10

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:


- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.


Nita J. Bolz
Scientific Director
State Breath Alcohol Program

Subscribed and sworn before me this 26th day of April, 2010.


(Notary Seal Stamp)
Carolyn M. Noland
Notary Public, State of Alaska
Commission Expires with Office

BT9 03-06



VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 30579 ✓

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130579 ✓

APRIL 06, 2010

OPERATOR'S NAME: BMB 4/14/10 CR/1349 4/6/10
RITALA
OPERATOR'S NUMBER: 3791
SUBJECT'S LAST NAME:
VERIFICATION OF CALIBRATION
SUBJECT'S FIRST NAME/MI :
REPORTED COLD BREATH TUBE
O.L. #: A
DEPT/AGENCY: ANCL
CASE/REPORT: A
TEST TYPE: V
ALCO TARGET VALUE: .082 ✓
ALCO S/N: 718493

--- BREATH ANALYSIS ---

.082 ADJUSTED FOR 29.62 in ✓
ALCO TARGET .081 20:52
BLANK TEST .000 20:53
INTERNAL STANDARD VERIFIED 20:54
ALCO TV 29.62 in BMB 4/14/10 .081 ✓ 20:54
BLANK TEST .000 20:55
SUBJECT SAMPLE .000 20:55
BLANK TEST .000 20:56
ALCO TV 29.64 in .082 ✓ 20:56
BLANK TEST .000 20:57

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130579

APRIL 06, 2010 ✓ CR/1349
TIME 20:46

--- DIAGNOSTIC CHECK --- 4/6/10

COMPUTER: OKAY
PROGRAM: OKAY
SOFTWARE DATE: 12/11/08
HEATERS
SAMPLE CHAMBER: 50c
BREATH TUBE: 40c
BAROMETER: 29.62 in
FLOW DETECTOR: OKAY
PUMP
HIGH SPEED: OKAY
DETECTOR: OKAY
FILTERS: OKAY
QUARTZ STANDARD: OKAY
CALIBRATION: OKAY

PRINTER TEST
!"#\$%&'()*+,-./0123456789:;<=>?@ABCDEFGHIJKL
MNOPQRSTUVWXYZ[\]^_`abcdefgijklmno
pqrstuvwxyz{|}~^