

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

JUL 23 2009

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	130579 ✓		
Name	David Nell	ID#	6520	Date	7-23-09 ✓
A Agency	ANCI	Phone #	786-8928		
Instrument Location	Anchorage Jail ✓				
B Alco S/N	X124669 ✓	Target Value	.081 ✓	High Pressure	200
Alco Test Values	.082 ✓	1 <sup>st</sup> Alco	.082 ✓	2 <sup>nd</sup> Alco	
Signature					
(OVER)					

CB  
7/27/09  
7/30/09

(Do Not write in the area below)

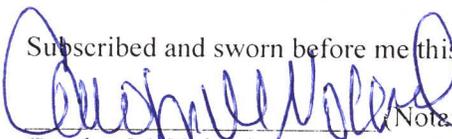
I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.



Nita J. Bolz  
Scientific Director  
State Breath Alcohol Program

Subscribed and sworn before me this 23 day of Aug, 2009

  
(Notary Seal Stamp)

Carolyn M. Noland  
Notary Public, State of Alaska  
Commission Expires with Office



# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130579 ✓

(CONTINUED FROM FRONT PAGE)

*Dadd*

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130579

JULY 23, 2009 ✓ *CSB 7/30/09*

OPERATOR'S NAME:  
NOLL

OPERATOR'S NUMBER: 6520

SUBJECT'S LAST NAME:

CALIBRATION

SUBJECT'S FIRST NAME/MI :

VERIFICATION/O

O.L. #: 012345

DEPT/AGENCY: ANC1

CASE/REPORT: 09-99999

TEST TYPE: V ✓

ALCO TARGET VALUE: .081 ✓

ALCO S/N: X124669 ✓

--- BREATH ANALYSIS ---

.081 ADJUSTED FOR 29.78 in  
ALCO TARGET .080  
BLANK TEST .000  
INTERNAL STANDARD VERIFIED  
ALCO TV 29.78 in .082 ✓  
BLANK TEST .000  
SUBJECT SAMPLE *CSB 7/30/09* .000  
BLANK TEST .000  
ALCO TV 29.78 in .082 ✓  
BLANK TEST .000

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130579

JULY 23, 2009  
TIME 01:55

*DN 30210 7-23-09*

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY  
PROGRAM: OKAY  
SOFTWARE DATE: 12/11/08  
HEATERS  
SAMPLE CHAMBER: 49c  
BREATH TUBE: 42c  
BAROMETER: 29.78 in  
FLOW DETECTOR: OKAY  
PUMP  
HIGH SPEED: OKAY  
DETECTOR: OKAY  
FILTERS: OKAY  
QUARTZ STANDARD: OKAY  
CALIBRATION: OKAY

PRINTER TEST

!"#\$%&'()\*+,-./0123456789:;<=>?@ABCDEFGHIJKL  
MNPQRSTUVWXYZ[\]^\_`abcdefghijklmnopqr  
stuvwxyz{|}~△