

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	130579 ✓		
Name	C. RITALA / 1349	ID#	3791	Date	7/24/08 ✓
A Agency	Anchorage P.D.	Phone #	786-2640		
Instrument Location	Anchorage Jail ✓				
B Alco S/N	57447 ✓	Target Value	.071 ✓	High Pressure	1100
Alco Test Values	.078 ✓ 1 <sup>st</sup> Alco		.079 ✓ 2 <sup>nd</sup> Alco		
Signature	Chris Ritala / 1349				CSB 7/25/08

(OVER)

Under the Alaska Rules of Evidence, I certify that;


(Do Not write in the area below)

(a) I am Jeanne Swartz, Forensic Scientist III, Scientific Crime Detection Laboratory, State of Alaska Department of Public Safety, and was, at the time of signing, the custodian of the records of the aforementioned laboratory and the signature was made in my official capacity as Scientific Director Designee of the State Breath Alcohol Testing Program.

(b) The verification of calibration for the above instrument has been received and reviewed. Instrument operator, Chris Ritala, whose name appears in my records, is qualified to verify the calibration of the above instrument.

(c) This instrument is certified for evidentiary use and these records are being retained as original documents in my custody.

Signed and sealed,

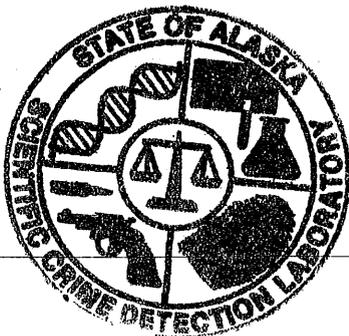

*Jeanne Swartz*

Jeanne Swartz  
Scientific Director Designee  
State of Alaska  
State Breath Alcohol Testing Program

7/28/08

Date

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N

130579 ✓

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

## DIAGNOSTIC CHECK

LASKA DEPARTMENT OF PUBLIC SAFETY  
ATAMASTER cdm 130579

JULY 24, 2008 ✓

OPERATOR'S NAME:

RITALA

OPERATOR'S NUMBER: 3791

SUBJECT'S LAST NAME:

VERIFICATION OF CALIBRATION

SUBJECT'S FIRST NAME/MI :

A

.L. #: A

EPT/AGENCY: ANC1

ASE/REPORT: A

TEST TYPE: V

LCO TARGET VALUE: .071 ✓

LCO S/N: 57447 ✓

### --- BREATH ANALYSIS ---

071 ADJUSTED FOR 29.83 in		
LCO TARGET	.070	17:25
BLANK TEST	.000	17:26
INTERNAL STANDARD	VERIFIED	17:26
LCO TV 29.83 in	.078 ✓	17:26
BLANK TEST	.000	17:27
SUBJECT SAMPLE	.000	17:27
BLANK TEST	.000	17:28
LCO TV 29.83 in	.079 ✓	17:29
BLANK TEST	.000	17:29

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130579

JULY 24, 2008 ✓

TIME 17:23

### --- DIAGNOSTIC CHECK ---

COMPUTER: OKAY

PROGRAM: OKAY

SOFTWARE DATE: 02/20/01

HEATERS

SAMPLE CHAMBER: 50c

BREATH TUBE: 41c

BAROMETER: 29.85 in

FLOW DETECTOR: OKAY

PUMP

HIGH SPEED: OKAY

DETECTOR: OKAY

FILTERS: OKAY

QUARTZ STANDARD: OKAY

CALIBRATION: OKAY

PRINTER TEST

!"#\$%&'()\*+,-./0123456789:;<=>?@ABCDEFGHIJKL  
HIJKLMNOPQRSTUVWXYZ[\]^\_`abcdefghijklmnopqr  
rstuvwxyz{|}

CR/1349

7/24/08

CR/1349

7/24/08