

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	<u>130579</u>
Name		<u>STEVE DUNN</u>	ID# <u>4106</u> Date <u>9-9-08</u> ✓
A	Agency	<u>APD</u>	Phone # <u>786-8900</u>
Instrument Location		<u>ANCHORAGE JAIL</u> ✓	
Alco S/N		<u>57023</u>	Target Value <u>.074</u> ✓ High Pressure <u>1200</u>
B	Alco Test Value Average	<u>.077</u> ✓	<u>.077</u> ✓
		1 <sup>st</sup> Alco	2 <sup>nd</sup> Alco
Signature			<u>COB</u> <u>9/12/08</u>
(OVER)			



Under the Alaska Rules of Evidence, I certify that:  
(Do Not write in the area below)

(a) I am Jeanne Swartz, Forensic Scientist III, Scientific Crime Detection Laboratory, State of Alaska Department of Public Safety, and was, at the time of signing, the custodian of the records of the aforementioned laboratory and the signature was made in my official capacity as Scientific Director Designee of the State Breath Alcohol Testing Program.

(b) The verification of calibration for the above instrument has been received and reviewed. Instrument operator, Steve P Dunn, whose name appears in my records, is qualified to verify the calibration of the above instrument.

(c) This instrument is certified for evidentiary use and these records are being retained as original documents in my custody.

Signed and sealed,

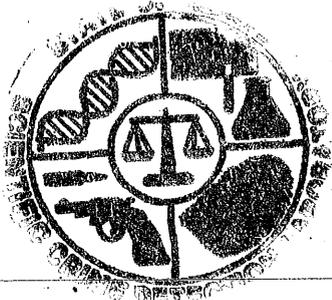

Jeanne Swartz  
Scientific Director Designee  
State of Alaska  
State Breath Alcohol Testing Program

9/15/08  
Date

SEP 11 2008

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N

130579 ✓

(CONTINUED FROM FRONT PAGE)

C

TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

*S. DUNN #1361*

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130579

SEPTEMBER 09, 2008 ✓ *sub*

OPERATOR'S NAME:

DUNN/S

OPERATOR'S NUMBER: 4106

SUBJECT'S LAST NAME:

VERIFICATION OF CAL

SUBJECT'S FIRST NAME/MI :

V

O.L. #: V

DEPT/AGENCY: ANC1

CASE/REPORT: V

TEST TYPE: V

ALCO TARGET VALUE: .074 ✓

ALCO S/N: 57023 ✓

--- BREATH ANALYSIS ---

.074 ADJUSTED FOR 29.70 in		
ALCO TARGET	.073	12:32
BLANK TEST	.000	12:33
INTERNAL STANDARD	VERIFIED	12:33
ALCO TV 29.70 in	.077 ✓	12:34
BLANK TEST	.000	12:35
SUBJECT SAMPLE	.000 <i>sub</i>	12:36
BLANK TEST	.000	12:36
ALCO TV 29.72 in	.077 ✓	12:37
BLANK TEST	.000	12:38

## DIAGNOSTIC CHECK

*S. DUNN #1361*

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130579

SEPTEMBER 09, 2008 ✓  
TIME 12:29

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY

PROGRAM: OKAY

SOFTWARE DATE: 02/20/01

HEATERS

SAMPLE CHAMBER: 49c

BREATH TUBE: 42c

BAROMETER: 29.70 in

FLOW DETECTOR: OKAY

PUMP

HIGH SPEED: OKAY

DETECTOR: OKAY

FILTERS: OKAY

QUARTZ STANDARD: OKAY

CALIBRATION: OKAY

PRINTER TEST

! "# % ' ( ) \* + , - . / 0 1 2 3 4 5 6 7 8 9 : ; < = > ? @ A B C D E F G  
H I J K L M N O P Q R S T U V W X Y Z [ \ ] ^ \_ ` a b c d e f g h i j k l m n o  
p q r s t u v w x y z { | } ~