

OCT 09 2009

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument  
State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

OCT 09 2009

Supervisor/Operator Performing the Verification Procedure:

DataMaster cdm S/N 130579 ✓

Name C. KRALA ID# 3791 Date 10/8/09 ✓

**A** Agency APD Phone # 786-2640

Instrument Location Anch Jail ✓

---

**B** Alco S/N X301563 ✓ Target Value .079 ✓ High Pressure 100

Alco Test Value Average 083 ✓ 083 ✓  
1<sup>st</sup> Alco 2<sup>nd</sup> Alco

Signature [Signature] 1349 ✓ 008  
10/12/09

(OVER)

(Do Not write in the area below)

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:


- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

[Signature]  
Nita J. Bolz  
Scientific Director  
State Breath Alcohol Program

Subscribed and sworn before me this 22<sup>nd</sup> day of Oct, 2009.

[Signature] (Notary Seal Stamp)

Carolyn M. Noland  
Notary Public, State of Alaska  
Commission Expires with Office



# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska


Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130579

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

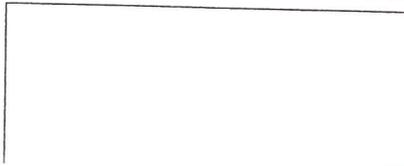

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130579

OCTOBER 08, 2009

OPERATOR'S NAME:

RITALA

OPERATOR'S NUMBER: 3791

SUBJECT'S LAST NAME:

VERIFICATION OF CALIBRATION

SUBJECT'S FIRST NAME/MI :

A

O.L. #: A

DEPT/AGENCY: ANCI

CASE/REPORT: A

TEST TYPE: V

ALCO TARGET VALUE: 079

ALCO S/N: X301563

--- BREATH ANALYSIS ---

.079 ADJUSTED FOR 30.20 in  
ALCO TARGET .079 22:31  
BLANK TEST .000 22:32  
INTERNAL STANDARD VERIFIED 22:32  
ALCO TV 30.20 in .083 22:32  
BLANK TEST .000 22:33  
SUBJECT SAMPLE .000 22:33  
BLANK TEST .000 22:34  
ALCO TV 30.20 in .083 22:35  
BLANK TEST .000 22:35

CR/1349 10/8/09



## DIAGNOSTIC CHECK



ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130579

OCTOBER 08, 2009  
TIME 22:30

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY  
PROGRAM: OKAY  
SOFTWARE DATE: 12/11/08  
HEATERS  
SAMPLE CHAMBER: 49c  
BREATH TUBE: 42c  
BAROMETER: 30.20 in  
FLOW DETECTOR: OKAY  
PUMP  
HIGH SPEED: OKAY  
DETECTOR: OKAY  
FILTERS: OKAY  
QUARTZ STANDARD: OKAY  
CALIBRATION: OKAY

PRINTER TEST

!"#\$%&'()\*+,-./0123456789:;<=>?@ABCDEFGHIJKL  
MNOPQRSTUVWXYZ[\]^\_`abcdefghijklmnopqrstuvwxyz{|}~Δ

CR/1349

10/8/09

