

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure:	
DataMaster cdm S/N <u>130579</u> ✓	
Name <u>Douglas S. Henie</u>	ID# <u>3554</u> ✓ Date <u>11-30-10</u> ✓
A Agency <u>APD</u>	Phone # <u>786-8500</u>
Instrument Location <u>Anchorage Jail</u>	
B Alco S/N <u>2X</u> ✓ Target Value <u>.080</u> ✓ High Pressure <u>1050</u>	
Alco Test Values <u>.079</u> ✓ <u>.080</u> ✓	
1 <sup>st</sup> Alco 2 <sup>nd</sup> Alco	
Signature <u>Douglas S. Henie</u>	

(OVER)

BMB  
12/16/10

(Do Not write in the area below)



I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

Nita J. Bolz  
Nita J. Bolz  
Scientific Director  
State Breath Alcohol Program

Subscribed and sworn before me this 5<sup>th</sup> day of JAN, 2011.

Daniel L. Nicholas (Notary Seal Stamp)  
Carolyn M. Noland DANIEL L. NICHOLAS  
Notary Public, State of Alaska  
Commission Expires with Office

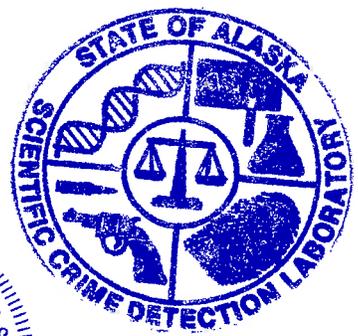

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130579

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130579

NOVEMBER 30, 2010

OPERATOR'S NAME: HENIE, DOUGLAS S  
OPERATOR'S NUMBER: 3554  
SUBJECT'S LAST NAME:  
TEST VOC  
SUBJECT'S FIRST NAME/MI :  
TEST VOC  
O.L. #: 1111111  
DEPT/AGENCY: ANC1  
CASE/REPORT: 000000  
TEST TYPE: T  
ALCO TARGET VALUE: .080  
ALCO S/N: 2X

### --- BREATH ANALYSIS ---

.080 ADJUSTED FOR 29.60 in  
ALCO TARGET .079 02:37  
BLANK TEST .000 02:38  
INTERNAL STANDARD VERIFIED 02:38  
ALCO TV 29.62 in .079 02:38  
BLANK TEST .000 02:39  
SUBJECT SAMPLE .000 02:39  
BLANK TEST .000 02:40  
ALCO TV 29.60 in .080 02:40  
BLANK TEST .000 02:41

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130579

NOVEMBER 30, 2010  
TIME 02:35

### --- DIAGNOSTIC CHECK ---

COMPUTER: OKAY  
PROGRAM: OKAY  
SOFTWARE DATE: 12/11/08  
HEATERS  
SAMPLE CHAMBER: 49c  
BREATH TUBE: 42c  
BAROMETER: 29.62 in  
FLOW DETECTOR: OKAY  
PUMP  
HIGH SPEED: OKAY  
DETECTOR: OKAY  
FILTERS: OKAY  
QUARTZ STANDARD: OKAY  
CALIBRATION: OKAY

### PRINTER TEST

!"#\$%&'()\*+,-./0123456789:;<=>?@ABCDEF  
GHIJKLMNOPQRSTUVWXYZ[\]^\_`abcdefg  
hijklmno pqrstuvwxyz{|}~Δ