


VERIFICATION OF CALIBRATION REPORT
of DataMaster cdm Breath Test Instrument
State of Alaska
Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N: 130584

Supervisor/Operator Performing the Verification Procedure:


Name Supt. James R. R. Rea ID# 3161 Date 02-11-12
A Agency Kotzebue Police Department Phone # 907-442-3352
 Instrument Location Kotzebue Regional Jail 258d rm#107 Fourth Avenue Kotzebue, AK 99752

Alco S/N 78890 ^{4F} <u>COB-264/12</u>	Target Value <u>.080</u>	High Pressure <u>0225</u>
Alco Test Values:		
B	<u>.077</u> 1 st Alco	<u>.075</u> 2 nd Alco
Signature 	Supt. James R. R. Rea (OVER)	 <u>2/24/12</u>


(Do Not write in the area below)


I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

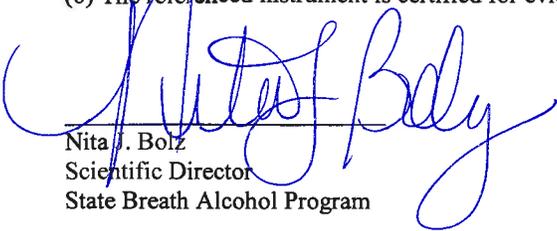
 Nita J. Bolz
 Scientific Director
 State Breath Alcohol Program

Subscribed and sworn before me this 5 day of April, 2012.

 (Notary Seal Stamp)
~~Daniel L. Nicholas~~ Nikki Roth
 Notary Public, State of Alaska
 Commission Expires with Office 4/5/12

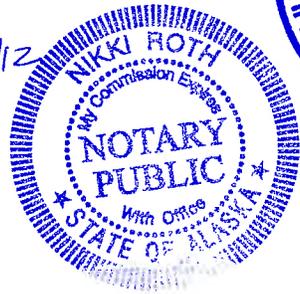

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130584

(CONTINUED FROM FRONT PAGE)

C

TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130584

FEBRUARY 11, 2012

OPERATOR'S NAME: REP/JAMES/RR *COB 2/24/12*

OPERATOR'S NUMBER: 0161

SUBJECT'S LAST NAME: VERIFICATION OF CAL

SUBJECT'S FIRST NAME/NI: VDC

O.L. #: 02-11-2011

DEPT/AGENCY: 0T21

CASE/REPORT: 02-11-2011

TEST TYPE: V

ALCO TARGET VALUE: .000

ALCO S/N: 4F

--- BREATH ANALYSIS ---

.000 ADJUSTED FOR 29.54 in		
ALCO TARGET	.078	14:19
BLANK TEST	.000	14:21
INTERNAL STANDARD	VERIFIED	14:21
ALCO TV 29.54 in	.077	14:21
BLANK TEST	.000	14:22
SUBJECT SAMPLE	.000	14:22
BLANK TEST	.000	14:23
ALCO TV 29.54 in	.075	14:23
BLANK TEST	.000	14:24

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130584

FEBRUARY 11, 2012
TIME 14:25

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY

PROGRAM: OKAY

SOFTWARE DATE: 02/20/01

HEATERS

SAMPLE CHAMBER: 50c

BREATH TUBE: 42c

BAROMETER: 29.54 in

FLOW DETECTOR: OKAY

PUMP

HIGH SPEED: OKAY

DETECTOR: OKAY

FILTERS: OKAY

QUARTZ STANDARD: OKAY

CALIBRATION: OKAY

PRINTER TEST

!"#\$%&'()*+,-./0123456789:;<=>?@ABCDEFGHIJKL
MNPQRSTUVWXYZ[\]^_`abcde fghijklmnop
qrstuvwxyz{|}~"