

**VERIFICATION OF CALIBRATION REPORT**  
*of DataMaster cdm Breath Test Instrument*  
*State of Alaska*  
*Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program*

**DataMaster cdm S/N: 130584** ✓

Supervisor/Operator Performing the Verification Procedure:

Name Supt. James R. R. Rea ID# 3161 Date 10-11-08 ✓

**A** Agency Kotzebue Police Department Phone # 907-442-3352

Instrument Location Kotzebue Regional Jail 258d rm#107 Fourth Avenue Kotzebue, AK 99752 ✓

Alco S/N X172931 ✓ Target Value .084 ✓ High Pressure 1275 ✓


Alco Test Values:

**B** .084 ✓ .085 ✓  
 1<sup>st</sup> Alco 2<sup>nd</sup> Alco

Signature \_\_\_\_\_ *[Signature]* Supt. James R. R. Rea  
 (OVER) *[Signature]* 11/29/08

(Do Not write in the area below)  
 Under the Alaska Rules of Evidence, I certify that,

- (a) I am Jeanne Swartz, Forensic Scientist III, Scientific Crime Detection Laboratory, State of Alaska Department of Public Safety, and was, at the time of signing, the custodian of the records of the aforementioned laboratory and the signature was made in my official capacity as Scientific Director Designee of the State Breath Alcohol Testing Program.
- (b) The verification of calibration for the above instrument has been received and reviewed. Instrument operator, James Rea, whose name appears in my records, is qualified to verify the calibration of the above instrument.
- (c) This instrument is certified for evidentiary use and these records are being retained as original documents in my custody.

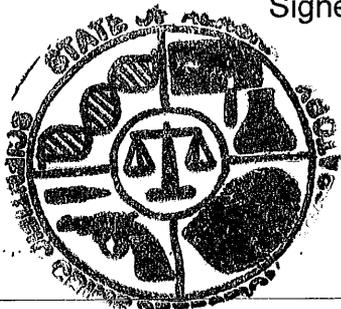

Signed and sealed,

*[Signature]* \_\_\_\_\_ *11/21/08*  
 Jeanne Swartz Date  
 Scientific Director Designee  
 State of Alaska  
 State Breath Alcohol Testing Program

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130584 ✓

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130584

OCTOBER 11, 2008 ✓ *COB 11/20/08*

OPERATOR'S NAME:  
REA/JAMES/RR  
OPERATOR'S NUMBER: 3161  
SUBJECT'S LAST NAME:  
VERIFICATION OF CAL  
SUBJECT'S FIRST NAME/MI :  
VERIFICATION OF CAL  
O.L. #: 10112008  
DEPT/AGENCY: OTZI  
CASE/REPORT: 10112008  
TEST TYPE: V  
ALCO TARGET VALUE: .004 ✓  
ALCO S/N: X172931

--- BREATH ANALYSIS ---

.004 ADJUSTED FOR 30.03 in

ALCO TARGET	.004	✓	19:34
BLANK TEST	.000		19:35
INTERNAL STANDARD	VERIFIED		19:35
ALCO TV 30.03 in	.004	✓	19:35
BLANK TEST	.000		19:36
SUBJECT SAMPLE	.000		19:36
BLANK TEST	.000		19:39
ALCO TV 30.03 in	.005	✓	19:39
BLANK TEST	.000		19:40

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130584

OCTOBER 11, 2008 ✓  
TIME 19:32

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY  
PROGRAM: OKAY  
SOFTWARE DATE: 02/20/01

HEATERS  
SAMPLE CHAMBER: 49c  
BREATH TUBE: 42c

BAROMETER: 30.03 in

FLOW DETECTOR: OKAY ✓

PUMP  
HIGH SPEED: OKAY

DETECTOR: OKAY  
FILTERS: OKAY  
QUARTZ STANDARD: OKAY  
CALIBRATION: OKAY

PRINTER TEST  
!"#\$%&'()\*+,-./0123456789:;<=>?@ABCDEFGHI  
JKLMNOPQRSTUVWXYZ[\]^\_`abcde fghijklmnop  
qrstuvwxyz{|}~