

**VERIFICATION OF CALIBRATION REPORT**  
*of DataMaster cdm Breath Test Instrument*  
*State of Alaska*  
**Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program**

**DataMaster cdm S/N: 130584**

Supervisor/Operator Performing the Verification Procedure:

Name Supt. James R. R. Rea

ID# 3161

Date 02-08-10

**A** Agency Kotzebue Police Department

Phone # 907-442-3352

Instrument Location Kotzebue Regional Jail 258d rm#107 Fourth Avenue Kotzebue, AK 99752

Alco S/N 78890

Target Value .082

High Pressure 1200

Alco Test Values:

**B**

.083  
1<sup>st</sup> Alco

.083  
2<sup>nd</sup> Alco

Signature \_\_\_\_\_



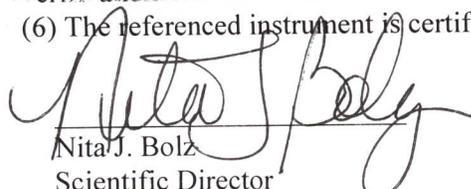
Supt. James R. R. Rea  
(OVER)

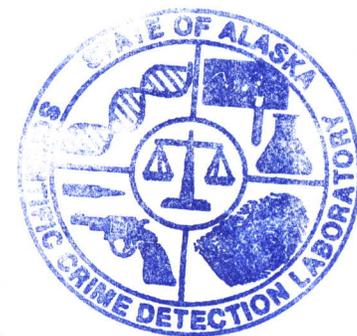
CRB  
3/11/10

(Do Not write in the area below)


I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

  
 Nita J. Bolz  
 Scientific Director  
 State Breath Alcohol Program



Subscribed and sworn before me this 23<sup>rd</sup> day of March, 2010.

 (Notary Seal Stamp)

Carolyn M. Noland  
 Notary Public, State of Alaska  
 Commission Expires with Office



# VERIFICATION OF CALIBRATION REPORT

*of DataMaster cdm breath Test Instrument*  
*State of Alaska*  
*Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program*

DataMaster cdm S/N 130584 ✓

(CONTINUED FROM FRONT PAGE)

**C** TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

### NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
 DATAMASTER cdm 130584 ✓

### DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
 DATAMASTER cdm 130584 ✓

#### Breath Test Record

Serial Number 130584 Model DataMaster  
 Location OTZ1 Kotzebue Police Dept.

311/10

#### Diagnostic Test Record

Serial Number 130584 Model DataMaster  
 Location OTZ1 Kotzebue Police Dept.

#### Subject Information

Last Name Verification Of Cal O.L. # 02082010  
 First Name Verification Of Cal

#### Operator Information

Operator Name Rea/James/Rr Case 02082010  
 Operator # 3161 Department OTZ1

#### Test Results

Alco Target	<u>082</u>	Alco Serial	<u>78890</u>
Nominal	<u>0.082</u>	Barometer	<u>30.17</u>
Dry Gas 1	<u>0.083</u>	Time:	<u>16:45:53</u>
Subject Alcohol	<u>0.000</u>	Time:	<u>16:47:49</u>
Dry Gas 2	<u>0.083</u>	Time:	<u>16:48:59</u>
		Test Type	<u>V</u>
		Test Date	<u>02/08/2010</u>
		Test Time	<u>16:44:09</u>
		Report	<u>Y</u>

#### Diagnostic Test Results

Test Date	<u>02/08/2010</u>	Computer	<u>Okay</u>
Test Time	<u>16:52:12</u>	Program	<u>Okay</u>
		Software Date	<u>02/20/2001</u>
		Sample Chamber (C)	<u>49</u>
		Breath Tube (C)	<u>41</u>
		Barometer (in)	<u>30.17</u>
		Flow Detector	<u>Okay</u>
		High Speed Pump	<u>Okay</u>
		Detector	<u>Okay</u>
		Filter	<u>Okay</u>
		Quartz	<u>Okay</u>
		Calibration	<u>Okay</u>

SUBJECT  
 ALCO 1V 30.17 in .000  
 BLANK TEST .000 16:49

CALIBRATION  
 0123456789;()=)@HJLDEFB  
 HIJKLNPQRSTUWXYZ\]^\_`abcde fghijklmno  
 pqrstuvwxyz{|}~