

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument
State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program MAR 23 2010

DataMaster cdm S/N: 130584

Supervisor/Operator Performing the Verification Procedure:

Name Supt. James R. R. Rea

ID# 3161

Date 03-17-10

A Agency Kotzebue Police Department

Phone # 907-442-3352

Instrument Location Kotzebue Regional Jail 258d rm#107 Fourth Avenue Kotzebue, AK 99752

Alco S/N 78890

Target Value .082

High Pressure 1200


Alco Test Values:

.083
1st Alco

.083
2nd Alco

B

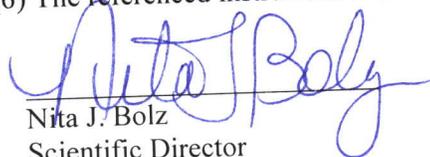
Signature _____


Supt. James R. R. Rea
(OVER)

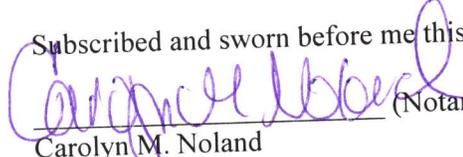
(Do Not write in the area below)

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.


Nita J. Bolz
Scientific Director
State Breath Alcohol Program

Subscribed and sworn before me this 15th day of April, 2010.


(Notary Seal Stamp)

Carolyn M. Noland
Notary Public, State of Alaska
Commission Expires with Office



VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130584

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130584 ✓

MARCH 17, 2010 ✓

OPERATOR'S NAME:

REA/JAMES/RR

OPERATOR'S NUMBER: 3161

SUBJECT'S LAST NAME:

VERIFICATION OF CAL

SUBJECT'S FIRST NAME/MI :

VERIFICATION OF CAL

O.L. #: 03172010

DEPT/AGENCY: 0T21

CASE/REPORT: 03172010

TEST TYPE: V

ALCO TARGET VALUE: 002 ✓

ALCO S/N: 78890 ✓

--- BREATH ANALYSIS ---

.082 ADJUSTED FOR 30.55 in

ALCO TARGET	.083	15:38
BLANK TEST	.000	15:39
INTERNAL STANDARD	VERIFIED	15:39
ALCO TV 30.55 in	.083 ✓	15:40
BLANK TEST	.000	15:41
SUBJECT SAMPLE	.000	15:41
BLANK TEST	.000	15:42
ALCO TV 30.55 in	.083 ✓	15:42
BLANK TEST	.000	15:43

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130584 ✓

MARCH 17, 2010 ✓

TIME 15:44

--- DIAGNOSTIC CHECK ---

COMPUTER:	OKAY
PROGRAM:	OKAY
SOFTWARE DATE:	02/20/01
HEATERS	
SAMPLE CHAMBER:	49c
BREATH TUBE:	40c
BAROMETER:	30.55 in
FLOW DETECTOR:	OKAY
PUMP	
HIGH SPEED:	OKAY
DETECTOR:	OKAY
FILTERS:	OKAY
QUARTZ STANDARD:	OKAY
CALIBRATION:	OKAY

PRINTER TEST

!@#%&'()*+,-./0123456789:;<=>?@ABCDEFG
HIJKLMNPOQRSTUVWXYZ[\]^_`abcde fghijklmno
pqrstuvwxy z{|}~