

# VERIFICATION OF CALIBRATION REPORT OCT 04 2010

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N: 130584 ✓

Supervisor/Operator Performing the Verification Procedure:

Name Supt. James R. R. Rea

ID# 3161 ✓

Date 09-25-10 ✓

A Agency Kotzebue Police Department

Phone # 907-442-3352

Instrument Location Kotzebue Regional Jail 258d rm#107 Fourth Avenue Kotzebue, AK 99752

Alco S/N 78890 ✓

Target Value .082 ✓

High Pressure 0550

B

Alco Test Values:

.082 ✓  
1<sup>st</sup> Alco

.083 ✓  
2<sup>nd</sup> Alco

Signature \_\_\_\_\_




Supt. James R. R. Rea  
(OVER)

BMB  
10/5/10

(Do Not write in the area below)


I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

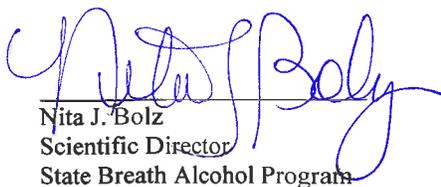  
Nita J. Bolz  
Scientific Director  
State Breath Alcohol Program

Subscribed and sworn before me this 16<sup>th</sup> day of DEC, 2010.

  
(Notary Seal Stamp)  
Daniel L. Nicholas  
Notary Public, State of Alaska  
Commission Expires with Office

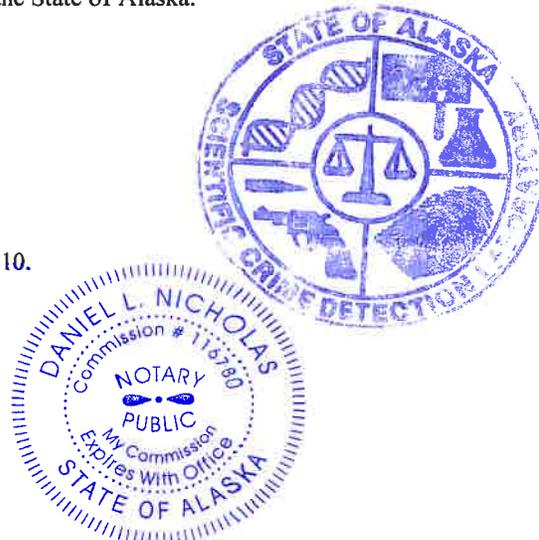

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130584

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130584

SEPTEMBER 25, 2010

OPERATOR'S NAME: *BMB*  
REA/NAES/RR  
OPERATOR'S NUMBER: 3161  
SUBJECT'S LAST NAME:  
VERIFICATION OF CAL  
SUBJECT'S FIRST NAME/MI :  
VOC  
O.L. #: 09252010  
DEPT/AGENCY: OT21  
CASE/REPORT: 09252010  
TEST TYPE: V  
ALCO TARGET VALUE: 002  
ALCO S/N: 78890

--- BREATH ANALYSIS ---

.002 ADJUSTED FOR 29.96 in  
ALCO TARGET .002 10:17  
BLANK TEST .000 10:18  
INTERNAL STANDARD VERIFIED 10:18  
ALCO TV 29.96 in .002 10:18  
BLANK TEST .000 10:19  
SUBJECT SAMPLE *BMB* .000 10:20  
BLANK TEST .000 10:20  
ALCO TV 29.98 in .003 10:21  
BLANK TEST .000 10:22

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130584

SEPTEMBER 25, 2010  
TIME 10:23

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY  
PROGRAM: OKAY  
SOFTWARE DATE: 02/20/01  
HEATERS  
SAMPLE CHAMBER: 49c  
BREATH TUBE: 41c  
BAROMETER: 29.98 in  
FLOW DETECTOR: OKAY  
PUMP  
HIGH SPEED: OKAY  
DETECTOR: OKAY  
FILTERS: OKAY  
QUARTZ STANDARD: OKAY  
CALIBRATION: OKAY

PRINTER TEST

!@#&'()\*+,-./0123456789:;<=>?@BCDEF6  
HIJKLMNOPQRSTUVWXYZ^\_`abcde:ghi.jklmno  
pqrstuvwxyz{|}~\*