

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure: DataMaster cdm S/N 130660 ✓

Name Garrett R. Willis ID# 5560 Date 3-9-11

A Agency AST Phone # 907-262-4453

Instrument Location Cooper Landing

B Alco S/N 57345 Target Value .082 ✓ High Pressure 650

Alco Test Value Average .084 ✓ .084 ✓
1st Alco 2nd Alco

Signature Garrett Willis

(OVER)

Handwritten initials and date:
DWB
3/31/11


I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

Handwritten signature of Nita J. Bolz
Nita J. Bolz
Scientific Director
State Breath Alcohol Program

Subscribed and sworn before me this 1st day of APRIL, 2011

Handwritten signature of Daniel L. Nicholas
(Notary Seal Stamp)
Daniel L. Nicholas
Notary Public, State of Alaska
Commission Expires with Office

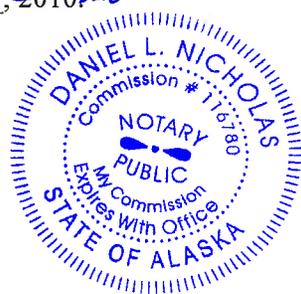

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130660

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130660

MARCH 09, 2011

OPERATOR'S NAME: *AMB 3/31/11*
WILLIS/GARRETT/R
OPERATOR'S NUMBER: 5560
SUBJECT'S LAST NAME:
VOC
SUBJECT'S FIRST NAME/MI :
VOC

O.L. #: VOC
DEPT/AGENCY: C000 *Liwi*
CASE/REPORT: VOC
TEST TYPE: V
ALCO TARGET VALUE: .002
ALCO S/N: 57345

--- BREATH ANALYSIS ---

.002 ADJUSTED FOR 29.52 in
ALCO TARGET .000 12:22
BLANK TEST .000 12:22
INTERNAL STANDARD VERIFIED 12:22
ALCO TV 29.52 in .004 12:23
BLANK TEST .000 12:23
SUBJECT SAMPLE *AMB 3/31/11* .000 12:24
BLANK TEST .000 12:25
ALCO TV 29.52 in .004 12:25
BLANK TEST .000 12:25

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130660

MARCH 09, 2011
TIME 12:19

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY
PROGRAM: OKAY
SOFTWARE DATE: 01/08/09 *Liwi*
HEATERS
SAMPLE CHAMBER: 49c
BREATH TUBE: 42c
BAROMETER: 29.52 in
FLOW DETECTOR: OKAY
PUMP
HIGH SPEED: OKAY
DETECTOR: OKAY
FILTERS: OKAY
QUARTZ STANDARD: OKAY
CALIBRATION: OKAY

PRINTER TEST

! " # \$ % & ' () * + , - . / 0 1 2 3 4 5 6 7 8 9 : ; < = > ? @ A B C D E F G
H I J K L M N O P Q R S T U V W X Y Z [\] ^ _ ` a b c d e f g h i j k l m n o
p q r s t u v w x y z { | } ~ () * + , - . / 0 1 2 3 4 5 6 7 8 9 : ; < = > ? @ A B C D E F G