


VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	130666
Name		Gary Yamamoto	ID# 2765 Date 02-20-2009
A	Agency	Fairbanks Police Department	Phone # 459-6500
Instrument Location		911 Cushman Street Fairbanks, Alaska 99701	
Alco S/N		X301737	Target Value .080 High Pressure 50
B	Alco Test Value Average	.084	.084
		1 st Alco	2 nd Alco
Signature			

(OVER)

Under the Alaska Rules of Evidence, I certify that;


(Do Not write in the area below)

(a) I am Jeanne Swartz, Forensic Scientist III, Scientific Crime Detection Laboratory, State of Alaska Department of Public Safety, and was, at the time of signing, the custodian of the records of the aforementioned laboratory and the signature was made in my official capacity as Scientific Director Designee of the State Breath Alcohol Testing Program.

(b) The verification of calibration for the above instrument has been received and reviewed. Instrument operator, Gary Yamamoto, whose name appears in my records, is qualified to verify the calibration of the above instrument.

(c) This instrument is certified for evidentiary use and these records are being retained as original documents in my custody.

Signed and sealed,

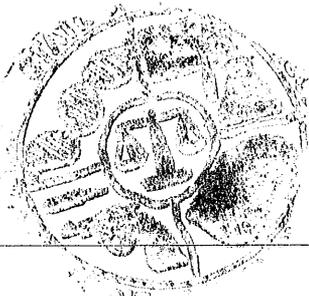



Jeanne Swartz
Scientific Director Designee
State of Alaska
State Breath Alcohol Testing Program

3/11/09

Date

VERIFICATION OF CALIBRATION REPORT

*of DataMaster cdm breath Test Instrument
State of Alaska
Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program*

DataMaster cdm S/N 130666 ✓

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130666

FEBRUARY 20, 2009

OPERATOR'S NAME: *COB 3/10/09*
YAMAMOTO
OPERATOR'S NUMBER: 2765
SUBJECT'S LAST NAME: *[Signature]*
VERIFICATION OF CAL
SUBJECT'S FIRST NAME/NI :
VOC

O.L. #: 1111
DEPT/AGENCY: FBK1
CASE/REPORT: 1111
TEST TYPE: V
ALCO TARGET VALUE: .000 ✓
ALCO S/N: X301737 ✓

--- BREATH ANALYSIS ---

02/11/09

.000 ADJUSTED FOR 30.20 in		
ALCO TARGET	.000	02:14
BLANK TEST	.000	02:15
INTERNAL STANDARD	VERIFIED	02:15
ALCO TV 30.20 in	.004 ✓	02:15
BLANK TEST	.000	02:16
SUBJECT SAMPLE	.000	02:17
BLANK TEST	.000	02:17
ALCO TV 30.20 in	.004 ✓	02:18
BLANK TEST	.000	02:18

COB 3/10/09

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130666

FEBRUARY 20, 2009 ✓
TIME 02:12

--- DIAGNOSTIC CHECK --- *[Signature]*

COMPUTER:	OKAY
PROGRAM:	OKAY
SOFTWARE DATE:	02/20/01
HEATERS	
SAMPLE CHAMBER:	50c
BREATH TUBE:	42c
BAROMETER:	30.20 in
FLOW DETECTOR:	OKAY
PUMP	
HIGH SPEED:	OKAY
DETECTOR:	OKAY
FILTERS:	OKAY
QUARTZ STANDARD:	OKAY
CALIBRATION:	OKAY

PRINTER TEST

! " # % & ' () * + , - . / 0 1 2 3 4 5 6 7 8 9 : ; < = > ? @ A B C D E F G
H I J K L M N O P Q R S T U V W X Y Z [\] ^ _ ` a b c d e f g h i j k l m n o
p q r s t u v w x y z { | } ~