

STATEMENT OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	<u>130666</u>
Name	<u>Matthew L. Soden</u>	ID#	<u>3378</u>
		Date	<u>3-5-2008</u>
A Agency		<u>Fairbanks Police Department</u>	Phone # <u>(907) 459-6500</u>
Instrument Location <u>911 Cushman St. Fairbanks, AK 99701</u>			
B Alco S/N		<u>X124617</u>	Target Value <u>.081</u>
		High Pressure	<u>1000</u>
Alco Test Values		<u>.079</u>	<u>.079</u>
	1 st Alco		2 nd Alco
Signature			

(OVER)


Under the Alaska Rules of Evidence, I certify that; (Do Not write in the area below)


(a) I am Jeanne Swartz, Forensic Scientist III, Scientific Crime Detection Laboratory, State of Alaska Department of Public Safety, and was, at the time of signing, the custodian of the records of the aforementioned laboratory and the signature was made in my official capacity as Scientific Director Designee of the State Breath Alcohol Testing Program.

(b) The verification of calibration for the above instrument has been received and reviewed. Instrument operator, Matthew Soden, whose name appears in my records, is qualified to verify the calibration of the above instrument.

(c) This instrument is certified for evidentiary use and these records are being retained as original documents in my custody.

Signed and sealed,

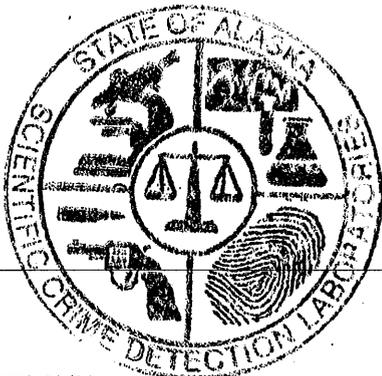



Jeanne Swartz
Scientific Director Designee
State of Alaska
State Breath Alcohol Testing Program

3/18/08
Date

STATEMENT OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Criminal Justice Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130666

(CONTINUED FROM FRONT PAGE)

C

TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130666

MARCH 05, 2008

OPERATOR'S NAME:

SODEN, MATTHEW L

OPERATOR'S NUMBER: 3378

SUBJECT'S LAST NAME:

VERIFICATION OF CAL

SUBJECT'S FIRST NAME/MI :

X

O.L. #: X

DEPT/AGENCY: FBK1

CASE/REPORT: X

TEST TYPE: V

ALCO TARGET VALUE: .081

ALCO S/N: X124617

--- BREATH ANALYSIS ---

.081 ADJUSTED FOR 29.21 in
ALCO TARGET .079 13:16
BLANK TEST .000 13:17
INTERNAL STANDARD VERIFIED 13:18
ALCO TV 29.21 in .079 13:18
BLANK TEST .000 13:19
SUBJECT SAMPLE .000 13:19
BLANK TEST .000 13:20
ALCO TV 29.21 in .079 13:20
BLANK TEST .000 13:21

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130666

MARCH 05, 2008

TIME 13:32

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY

PROGRAM: OKAY

SOFTWARE DATE: 02/20/01

HEATERS
SAMPLE CHAMBER: 50c
BREATH TUBE: 42c

BAROMETER: 29.21 in

FLOW DETECTOR: OKAY

PUMP
HIGH SPEED: OKAY

DETECTOR: OKAY

FILTERS: OKAY

QUARTZ STANDARD: OKAY

CALIBRATION: OKAY

PRINTER TEST

!"#\$%&'()*+,-./0123456789:;<=>?@ABCDEFGHIJ
KLMNOPQRSTUVWXYZ[\]^_`abcde fghijklmno
pqrstuvwxyz{|}~