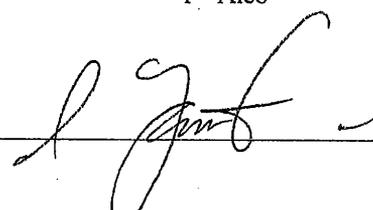



VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	130666
Name		Gary Yamamoto	ID# 2765 Date 10-23-08
A	Agency	Fairbanks Police Department	Phone # 459-6500
Instrument Location 911 Cushman Street Fairbanks, Alaska 99701			
Alco S/N		X172946	Target Value .077 High Pressure 850
B	Alco Test Value Average	.079	.079
		1 st Alco	2 nd Alco
Signature			

(OVER)


Under the Alaska Rules of Evidence, I certify that;

(Do Not write in the area below)


(a) I am Jeanne Swartz, Forensic Scientist III, Scientific Crime Detection Laboratory, State of Alaska Department of Public Safety, and was, at the time of signing, the custodian of the records of the aforementioned laboratory and the signature was made in my official capacity as Scientific Director Designee of the State Breath Alcohol Testing Program.

(b) The verification of calibration for the above instrument has been received and reviewed. Instrument operator, Gary Yamamoto, whose name appears in my records, is qualified to verify the calibration of the above instrument.

(c) This instrument is certified for evidentiary use and these records are being retained as original documents in my custody.

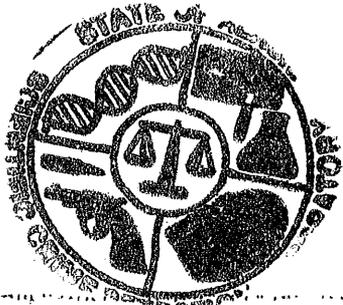

Signed and sealed



Jeanne Swartz
Scientific Director Designee
State of Alaska
State Breath Alcohol Testing Program

11/20/08

Date

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130666

(CONTINUED FROM FRONT PAGE)

C

TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130666

OCTOBER 23, 2008

OPERATOR'S NAME:

YAMAMOTO

OPERATOR'S NUMBER: 2765

SUBJECT'S LAST NAME:

VERIFICATION OF CAL

SUBJECT'S FIRST NAME/MI :

VOC

O.L. #: 1111

DEPT/AGENCY: FBK1

CASE/REPORT: 1111

TEST TYPE: V

ALCO TARGET VALUE: .077 ✓

ALCO S/N: X172946

--- BREATH ANALYSIS ---

.077 ADJUSTED FOR 29.36 in

ALCO TARGET	.075	03:50
BLANK TEST	.000	03:51
INTERNAL STANDARD	VERIFIED	03:51
ALCO TV 29.36 in	.079 ✓	03:52
BLANK TEST	.000	03:53
SUBJECT SAMPLE	.000	03:53
BLANK TEST	.000	03:54
ALCO TV 29.36 in	.079 ✓	03:54
BLANK TEST	.000	03:55

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130666

OCTOBER 23, 2008

TIME 03:47

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY

PROGRAM: OKAY

SOFTWARE DATE: 02/20/01

HEATERS

SAMPLE CHAMBER: 49c

BREATH TUBE: 41c

BAROMETER: 29.36 in

FLOW DETECTOR: OKAY

PUMP

HIGH SPEED: OKAY

DETECTOR: OKAY

FILTERS: OKAY

QUARTZ STANDARD: OKAY

CALIBRATION: OKAY

PRINTER TEST

!\"#%&'()*+,-./0123456789:;<=>?@ABCDEFGHIJKL
MNPQRSTUVWXYZ[\]^_`abcde fghijklmno
pqrstuvwxyz{|}~