


VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument
State of Alaska

JUL 19 2010

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

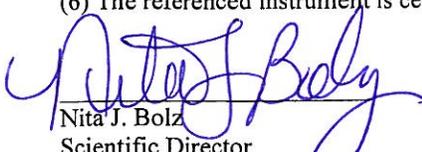
Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	130666 ✓
Name	Burlyn C. Rigdon Jr.	ID#	4154 ✓
		Date	07/13/2010 ✓
A	Agency	Fairbanks Police Department	Phone # (907) 450-6500
	Instrument Location	911 Cushman Street Fairbanks, AK 99701	
B	Alco S/N	X124611 ✓	Target Value .082 ✓
			High Pressure 1300 psi
	Alco Test Values	.083 ✓	.083 ✓
		1 st Alco	2 nd Alco
	Signature		
			CQB 7/19/10

(OVER)

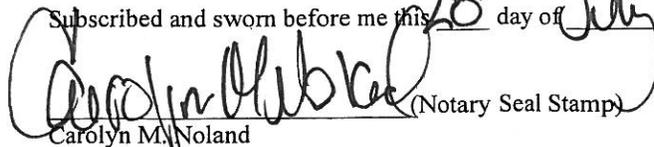
(Do Not write in the area below)

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.


Nita J. Bolz
Scientific Director
State Breath Alcohol Program

Subscribed and sworn before me this 28th day of July, 2010.


(Notary Seal Stamp)
Carolyn M. Noland
Notary Public, State of Alaska
Commission Expires with Office



VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130666

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

F

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130666

JULY 13, 2010

OPERATOR'S NAME:

RIGDON BURLYN C

OPERATOR'S NUMBER: 4154

SUBJECT'S LAST NAME:

VOC

SUBJECT'S FIRST NAME/MI :

VOC

O.L. #: 0000

DEPT/AGENCY: FBK1

CASE/REPORT: 0000

TEST TYPE: V

ALCO TARGET VALUE: .082

ALCO S/N: X124611

--- BREATH ANALYSIS ---

.082 ADJUSTED FOR 29.57 in
ALCO TARGET .081 20:16
BLANK TEST .000 20:17
INTERNAL STANDARD VERIFIED 20:17
ALCO TV 29.57 in .083 20:18
BLANK TEST .000 20:19
SUBJECT SAMPLE .000 20:19
BLANK TEST .000 20:20
ALCO TV 29.57 in .083 20:20
BLANK TEST .000 20:21

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130666

JULY 13, 2010

TIME 20:14

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY

PROGRAM: OKAY

SOFTWARE DATE: 02/20/01

HEATERS

SAMPLE CHAMBER: 49c

BREATH TUBE: 41c

BAROMETER: 29.57 in

FLOW DETECTOR: OKAY

PUMP

HIGH SPEED: OKAY

DETECTOR: OKAY

FILTERS: OKAY

QUARTZ STANDARD: OKAY

CALIBRATION: OKAY

PRINTER TEST

! " # % & ' () * + , - . / 0 1 2 3 4 5 6 7 8 9 : ; < = > ? @ A B C D E F G
H I J K L M N O P Q R S T U V W X Y Z I \] ^ _ ` a b c d e f g h i j k l m n o
p q r s t u v w x y z { | } ~