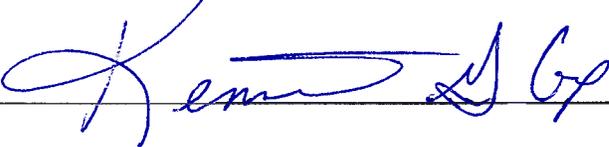


# VERIFICATION OF CALIBRATION REPORT

*of DataMaster cdm Breath Test Instrument  
State of Alaska*

*Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program*


DataMaster cdm S/N <u>130113</u>	
Supervisor/Operator Performing the Verification Procedure:	
Name	<u>Kenneth G. Cox</u> ID# <u>3527</u> Date <u>11/6/2011</u>
A Agency	<u>Skagway Police Department</u> Phone # <u>(907) 983-2232</u>
Instrument Location <u>Skagway Police Department 1st and State Street Skagway, AK 99840</u>	
B Alco S/N <u>X173019</u> Target Value <u>.082</u> High Pressure <u>500 psi</u>	
Alco Test Values	<u>.079</u> <u>.080</u> 1st Alco 2nd Alco
Signature	
(OVER)	

*DMB  
9/11/11*


(Do Not write in the area below)



I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

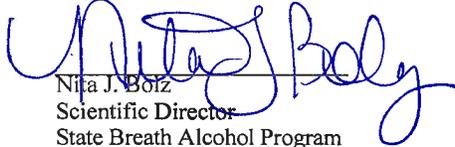  
Nita J. Bolz  
Scientific Director  
State Breath Alcohol Program

Subscribed and sworn before me this 1<sup>st</sup> day of Feb, 2011.

  
(Notary Seal Stamp)  
Daniel L. Nicholas  
Notary Public, State of Alaska  
Commission Expires with Office

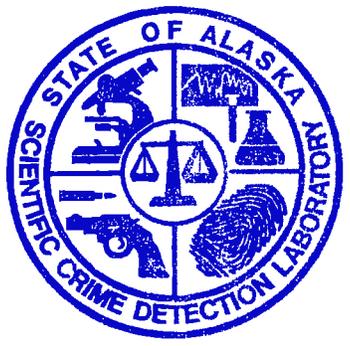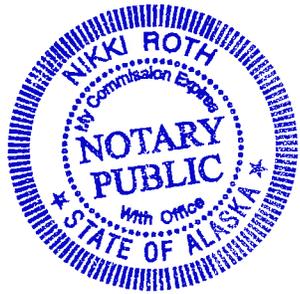

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument  
State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N

130113

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130113

NOVEMBER 06, 2011

OPERATOR'S NAME:  
COX/KENNETH/G  
OPERATOR'S NUMBER: 3527  
SUBJECT'S LAST NAME:  
VERIFICATION OF CAL  
SUBJECT'S FIRST NAME/MI :

L  
O.L. #: L  
DEPT/AGENCY: SKG1  
CASE/REPORT: 2011-0000  
TEST TYPE: U  
ALCO TARGET VALUE: .002  
ALCO S/N: X173019

### — BREATH ANALYSIS —

.002 ADJUSTED FOR 29.57 in  
ALCO TARGET .001 15:25  
BLANK TEST .000 15:26  
INTERNAL STANDARD VERIFIED 15:26  
ALCO TV 29.57 in .079 15:27  
BLANK TEST .000 15:28  
SUBJECT SAMPLE .000 15:28  
BLANK TEST .000 15:29  
ALCO TV 29.57 in .000 15:30  
BLANK TEST .000 15:30

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130113

NOVEMBER 06, 2011  
TIME 15:22

### — DIAGNOSTIC CHECK —

COMPUTER: OKAY  
PROGRAM: OKAY  
SOFTWARE DATE: 02/20/01  
HEATERS  
SAMPLE CHAMBER: 48c  
BREATH TUBE: 42c  
BAROMETER: 29.55 in  
FLOW DETECTOR: OKAY  
PUMP  
HIGH SPEED: OKAY  
DETECTOR: OKAY  
FILTERS: OKAY  
QUARTZ STANDARD: OKAY  
CALIBRATION: OKAY

### PRINTER TEST

!"#\$%&'()\*+,-./0123456789:;<=>?@ABCDEF6  
HIJKLMNOPQRSTUVWXYZ[\]^\_`abcdefgijklmno  
pqrs tuvxyz{|}~

