

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure: DataMaster cdm S/N 130115 ✓

Name Kevin Oldham ID# 5227 Date 7/21/08

A Agency Bristol Bay Borough PD Phone # 246-4222

Instrument Location Kings Salmon ✓

B Alco S/N X172961 ✓ Target Value 1.082 ✓ High Pressure 100

Alco Test Value Average 1.082 ✓ 1.084 ✓

1st Alco 2nd Alco


Signature Kevin Oldham CSB
Under Alaska Rules of Evidence, I certify that, 7/25/08

(a) ~~Jeane Swartz~~ ^(OVER) Jeane Swartz, Forensic Scientist III, Scientific Crime Detection Laboratory, State of Alaska Department of Public Safety, and was, at the time of signing, the custodian of the records of the aforementioned laboratory and the signature was made in my official capacity as Scientific Director Designee of the State Breath Alcohol Testing Program.

(b) The verification of calibration for the above instrument has been received and reviewed. Instrument operator, Kevin Oldham, whose name appears in my records, is qualified to verify the calibration of the above instrument.

(c) This instrument is certified for evidentiary use and these records are being retained as original documents in my custody.

Signed and sealed,

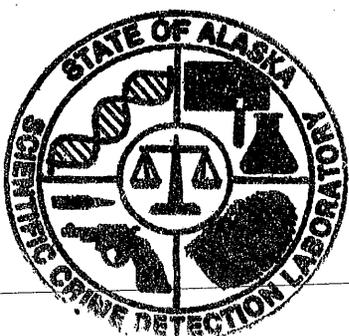

Jeane Swartz 7/28/08
Date
Jeane Swartz
Scientific Director Designee
State of Alaska
State Breath Alcohol Testing Program

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130115 ✓

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130115

JULY 21, 2008

OPERATOR'S NAME:

OLDHAM JAMES KEVIN

OPERATOR'S NUMBER: 5227

SUBJECT'S LAST NAME:

VOC

SUBJECT'S FIRST NAME/MI:

VOC

O.L. #: VOC

DEPT/AGENCY: NIKNI

CASE/REPORT: VOC

TEST TYPE: V

ALCO TARGET VALUE: .082 ✓

ALCO S/N: X172961 ✓

--- BREATH ANALYSIS ---

.082 ADJUSTED FOR 29.86 in
ALCO TARGET .081 14:21
BLANK TEST .000 14:22
INTERNAL STANDARD VERIFIED 14:22
ALCO TV 29.86 in .082 ✓ 14:22
BLANK TEST .000 14:23
SUBJECT SAMPLE .000 14:24
BLANK TEST .000 14:24
ALCO TV 29.86 in .084 14:25
BLANK TEST .000 14:26

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130115

JULY 21, 2008 ✓

TIME 14:19

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY

PROGRAM: OKAY

SOFTWARE DATE: 02/20/01

HEATERS

SAMPLE CHAMBER: 50c

BREATH TUBE: 40c

BAROMETER: 29.85 in

FLOW DETECTOR: OKAY

PUMP

HIGH SPEED: OKAY

DETECTOR: OKAY

FILTERS: OKAY

QUARTZ STANDARD: OKAY

CALIBRATION: OKAY

PRINTER TEST

!@%&'()*+,-./0123456789:;<=>?@ABCDEF
GHIJKLMNOPQRSTUVWXYZ[\]^_`abcde fghijklmno
pqrstuvwxyz{|}~