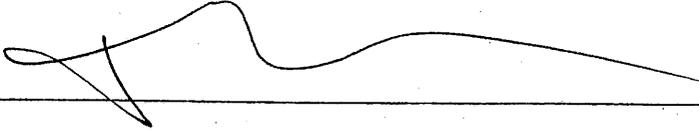


# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

|  |   |  |
|--|---|--|
| Supervisor/Operator Performing the Verification Procedure:                                   |   | DataMaster cdm S/N <u>130119</u>                   |
| Name <u>Tobin P Brennan</u>  |   | ID# <u>4542</u> Date <u>7-23-08</u>                |
| A  | Agency <u>Soldotna Police Department</u>              | Phone # <u>262-4455</u>                            |
|  | Instrument Location <u>Soldotna Police Department</u> |  |
| Alco S/N <u>X172933</u>  |   | Target Value <u>.082</u> High Pressure <u>1300</u> |
| B  | Alco Test Value Average <u>.083</u>                   | <u>.082</u>  |
|  | 1 <sup>st</sup> Alco                                  | 2 <sup>nd</sup> Alco                               |
| Signature  |   | <u>CS</u><br><u>7/30/08</u>                        |

(OVER)


Under the Alaska Rules of Evidence, I certify that,

(Do Not write in the area below)


(a) I am Jeanne Swartz, Forensic Scientist III, Scientific Crime Detection Laboratory, State of Alaska Department of Public Safety, and was, at the time of signing, the custodian of the records of the aforementioned laboratory and the signature was made in my official capacity as Scientific Director Designee of the State Breath Alcohol Testing Program.

(b) The verification of calibration for the above instrument has been received and reviewed. Instrument operator, Tobin P Brennan, whose name appears in my records, is qualified to verify the calibration of the above instrument.

(c) This instrument is certified for evidentiary use and these records are being retained as original documents in my custody.

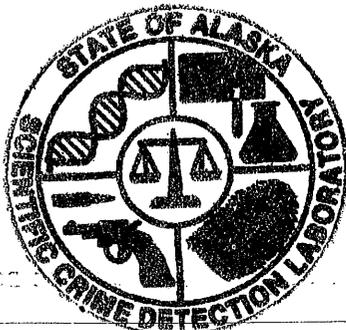

Signed and sealed,



Jeanne Swartz  
Scientific Director Designee  
State of Alaska  
State Breath Alcohol Testing Program

7/30/08  
Date

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130119

(CONTINUED FROM FRONT PAGE)

**C** TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130119

JULY 23, 2008

OPERATOR'S NAME:

BRENNAN

OPERATOR'S NUMBER: 4542

SUBJECT'S LAST NAME:

VERIFICATION OF CAL

SUBJECT'S FIRST NAME/NI :

UOC

O.L. #: UOC

DEPT/AGENCY: SLD1

CASE/REPORT: UOC

TEST TYPE: U

ALCO TARGET VALUE: .002 ✓

ALCO S/N: X172933 ✓

### --- BREATH ANALYSIS ---

.002 ADJUSTED FOR 29.00 in  
ALCO TARGET .001 02:51  
BLANK TEST .000 02:52  
INTERNAL STANDARD VERIFIED 02:52  
ALCO TO 29.00 in .003 02:52  
BLANK TEST .000 02:53  
SUBJECT SAMPLE .000 02:54  
BLANK TEST .000 02:54  
ALCO TO 29.00 in .002 02:55  
BLANK TEST .000 02:55

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130119

JULY 23, 2008

TIME 02:12

### --- DIAGNOSTIC CHECK ---

COMPUTER: OKAY  
PROGRAM: OKAY  
SOFTWARE DATE: 03/29/00  
HEATERS  
SAMPLE CHAMBER: 49c  
BREATH TUBE: 44c  
BAROMETER: 29.00 in  
FLOW DETECTOR: OKAY  
PUMP  
HIGH SPEED: OKAY  
DETECTOR: OKAY  
FILTERS: OKAY  
QUARTZ STANDARD: OKAY  
CALIBRATION: OKAY

### PRINTER TEST

!\*"#\$%&'()\*+,-./0123456789:;<=>?@ABCDEF  
HIJKL NOPQRSTU VWXYZ \]^\_` abcdefghijklmno  
pqrstuvwxyz{|}~@