

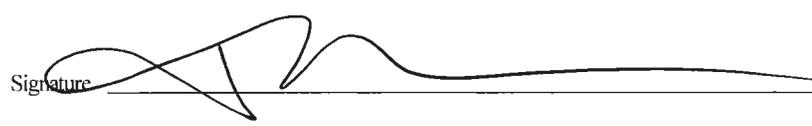
DEC 09 2010

# VERIFICATION OF CALIBRATION REPORT

*of DataMaster cdm Breath Test Instrument*

*State of Alaska*

*Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program*

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	<u>130119</u> ✓
Name	<u>Robin Brennan</u>	ID#	<u>4542</u> ✓
Date	<u>11-17-10</u> ✓		
A Agency	<u>Soldotna Police Dept</u>		Phone # <u>262-4455</u>
Instrument Location	<u>Soldotna Police Dept</u>		
B Alco S/N	<u>X301536</u> ✓	Target Value	<u>.081</u> ✓
		High Pressure	<u>1100</u>
Alco Test Values	<u>.085</u> ✓ 1st Alco	<u>.085</u> ✓ 2 <sup>nd</sup> Alco	
Signature			

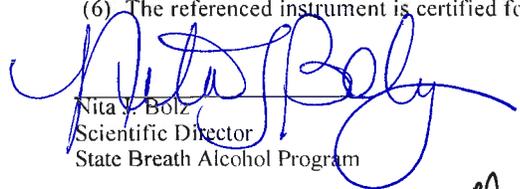
(OVER)

*AMB*  
*12/16/10*


(Do Not write in the area below)

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

  
 Nita J. Bolz  
 Scientific Director  
 State Breath Alcohol Program

Subscribed and sworn before me this 23<sup>rd</sup> day of DEC, 2010.

  
 (Notary Seal Stamp)  
 Daniel L. Nicholas  
 Notary Public, State of Alaska  
 Commission Expires with Office



# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130119

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130119

NOVEMBER 17, 2010

OPERATOR'S NAME: BRENNAN  
OPERATOR'S NUMBER: 4542  
SUBJECT'S LAST NAME: VERIFICATION OF CAL  
SUBJECT'S FIRST NAME/MI: NUC  
ALCO #1: NUC  
DEPT AGENCY: SLD1  
CASE REPORT: NUC  
TEST TYPE: U  
ALCO TARGET VALUE: .081  
ALCO S/N: XT01536

### --- BREATH ANALYSIS ---

.081 ADJUSTED FOR 30.64 in  
ALCO TARGET .082 15:40  
BLANK TEST .000 15:41  
INTERNAL STANDARD VERIFIED 15:41  
ALCO TO 30.64 in .085 15:41  
BLANK TEST .000 15:42  
SUBJECT SAMPLE .000 15:42  
BLANK TEST .000 15:43  
ALCO TO 30.64 in .085 15:44  
BLANK TEST .000 15:44

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130119

NOVEMBER 17, 2010  
TIME 15:45

### --- DIAGNOSTIC CHECK ---

COMPUTER: OKAY  
PROGRAM: OKAY  
SOFTWARE DATE: 07/28/09  
HEATERS  
SAMPLE CHAMBER: 49c  
BREATH TEST: 45c  
BAROMETER: 30.64 in  
FLOW DETECTOR: OKAY  
FLOW  
HIGH SPEED: OKAY  
DETECTOR: OKAY  
FILTERS: OKAY  
QUARTZ STANDARD: OKAY  
CALIBRATION: OKAY

### PRINTER TEST

ALCO #1: NUC  
TEST TYPE: U  
CASE REPORT: NUC  
DEPT AGENCY: SLD1