

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument
State of Alaska

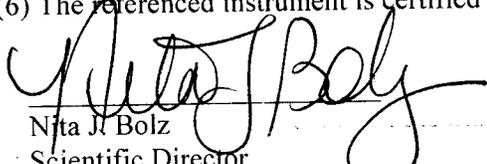
Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DEC 10 2009

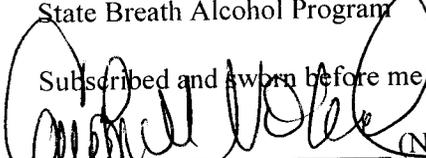
Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	130121 ✓			
Name	John Pernell	ID#	6260			
		Date	12/7/09 ✓			
A	Agency	Fairbanks Airport Police	Phone # 474-2555			
	Instrument Location	5795 Brumbaugh Fairbanks, AK 99709 ✓				
Alco S/N		57447 ✓	Target Value	.079 ✓	High Pressure	250
B	Alco Test Values		.082 ✓	.082 ✓		
		1 st Alco		2 nd Alco		
Signature		John Pernell ✓		SMB 12/31/09		
(OVER)						

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:


- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.


Nita J. Bolz
Scientific Director
State Breath Alcohol Program

Subscribed and sworn before me this 7th day of May, 2009.


(Notary Seal Stamp)

Carolyn M. Noland
Notary Public, State of Alaska
Commission Expires with Office



VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130121 ✓

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130121

DECEMBER 07, 2009 ✓

OPERATOR'S NAME: *BMB 12/31/09*
PERNELL/JOHN/T
OPERATOR'S NUMBER: 6260
SUBJECT'S LAST NAME:

UOC
SUBJECT'S FIRST NAME/MI :
UOC

O.L. #: UOC
DEPT/AGENCY: FBK6
CASE/REPORT: UOC
TEST TYPE: U
ALCO TARGET VALUE: .079 ✓
ALCO S/N: 57447 ✓

--- BREATH ANALYSIS ---

.079 ADJUSTED FOR 30.46 in
ALCO TARGET .000 07:03
BLANK TEST .000 07:04
INTERNAL STANDARD VERIFIED 07:04
ALCO TU 30.48 in .002 ✓ 07:05
BLANK TEST .000 07:05
SUBJECT SAMPLE *BMB 12/31/09* .000 07:06
BLANK TEST .000 07:07
ALCO TU 30.46 in .002 ✓ 07:07
BLANK TEST .000 07:08

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130121

DECEMBER 07, 2009 ✓
TIME 07:00

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY
PROGRAM: OKAY
SOFTWARE DATE: 03/29/00
HEATERS
SAMPLE CHAMBER: 48c
BREATH TUBE: 44c
BAROMETER: 30.46 in
FLOW DETECTOR: OKAY
PUMP
HIGH SPEED: OKAY
DETECTOR: OKAY
FILTERS: OKAY
QUARTZ STANDARD: OKAY
CALIBRATION: OKAY

PRINTER TEST

!"#\$%&'()*+,-./0123456789:;<=>?@AB0DEF6
HIJKL^HOPQRSTUUVWXYZ\]^_`abode"ghijklmno
pqrstuvwxyz{|}~■