

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

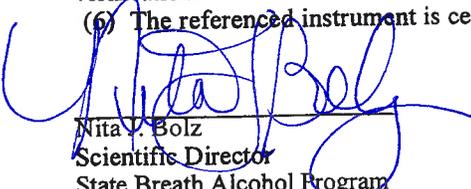
Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	<u>130127</u>
Name		<u>Christopher UmbS</u>	ID# <u>3669</u> Date <u>7/1/11</u>
A	Agency	<u>Alaska State Troopers</u>	Phone # <u>465-4004</u>
Instrument Location		<u>Angoon</u>	
Alco S/N		<u>70034</u>	Target Value <u>.079</u> High Pressure <u>150psi</u>
B	Alco Test Values	<u>.081</u> 1 <sup>st</sup> Alco	<u>.081</u> 2 <sup>nd</sup> Alco
Signature			
(OVER)			

*UMB*  
*7/1/11*


(Do Not write in the area below)

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:


- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

  
Nita J. Bolz  
Scientific Director  
State Breath Alcohol Program

Subscribed and sworn before me this 22 day of July, 2010. *2011* *1508*

 (Notary Seal Stamp)  
Daniel L. Nicholas *Nikki Roth*  
Notary Public, State of Alaska  
Commission Expires with Office

BT9 06/03



# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N

130127 <sup>BMB</sup> 7/11/11

(CONTINUED FROM FRONT PAGE)

C

TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130127

JULY 01, 2011

OPERATOR'S NAME: <sup>BMB</sup>  
UHBS/CHRISTOPHER/J  
OPERATOR'S NUMBER: 3669  
SUBJECT'S LAST NAME:

VOC  
SUBJECT'S FIRST NAME/MI :  
VOC

O.L. #: VOC  
DEPT/AGENCY: ASTO  
CASE/REPORT: VOC  
TEST TYPE: U  
ALCO TARGET VALUE: .079  
ALCO S/N: 70034

### --- BREATH ANALYSIS ---

.079 ADJUSTED FOR 29.85 in		
ALCO TARGET	.078	07:18
BLANK TEST	.000	07:20
INTERNAL STANDARD	VERIFIED	07:20
ALCO TV 29.83 in	.081	07:20
BLANK TEST	.000	07:21
SUBJECT SAMPLE	.000	07:21
BLANK TEST	.000	07:22
ALCO TV 29.83 in	.081	07:22
BLANK TEST	.000	07:23

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130127

JULY 01, 2011  
TIME 07:18

### --- DIAGNOSTIC CHECK ---

COMPUTER: OKAY  
PROGRAM: OKAY  
SOFTWARE DATE: 01/08/09  
HEATERS  
SAMPLE CHAMBER: 49c  
BREATH TUBE: 41c  
BAROMETER: 29.85 in  
FLOW DETECTOR: OKAY  
PUMP  
HIGH SPEED: OKAY  
DETECTOR: OKAY  
FILTERS: OKAY  
QUARTZ STANDARD: OKAY  
CALIBRATION: OKAY

### PRINTER TEST

!"#\$%&'()\*+,-./0123456789:;<=>?@ABCDEF6  
HIJKLMNPOQRSTUVWXYZ\]^\_`abcdefgijklmno  
pqrstuvwxyz{|}~||

