


# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N <u>130128</u> ✓
Name	<u>MALIK JONES</u>	ID# <u>5830</u> ✓ Date <u>1/25/11</u> ✓
A Agency	<u>AST</u>	Phone <u>(907) 451-5100</u>
Instrument Location <u>CANTWELL</u>		
B Alco S/N	<u>58442</u> <sup>043</sup> <u>130578</u> <sup>2/4/11</sup>	Target Value <u>.080</u> ✓ High Pressure <u>900 PSI</u>
Alco Test Values	<u>74</u> <sup>0.074</sup> <u>3/14/11</u> <sup>NFB</sup> <u>74</u> <sup>0.074</sup> <u>3/14/11</u> <sup>NFB</sup>	
Signature		
(OVER)		


VERIFIED CORRECT  
ALCO SN VIA  
EMAIL 2/4/11/BN  
AS PER MALIK JONES.

(Do Not write in the area below)

8MB  
3/6/11



I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

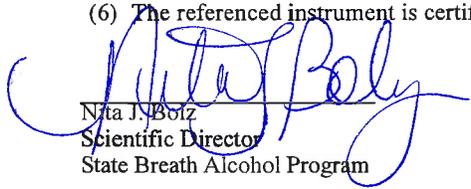  
Nita J. Bolz  
Scientific Director  
State Breath Alcohol Program

Subscribed and sworn before me this 14<sup>th</sup> day of MAR, 2011

  
(Notary Seal Stamp)  
Daniel L. Nicholas  
Notary Public, State of Alaska  
Commission Expires with Office

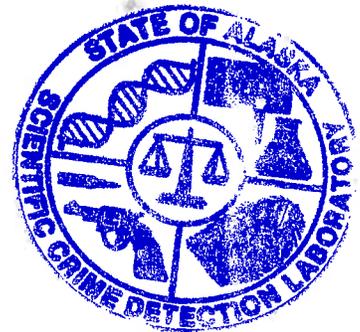

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument  
State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N

130128 *BMB*  
3/6/11

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130128

JANUARY 25, 2011

OPERATOR'S NAME:

JONES/MALIK/JAMAL

OPERATOR'S NUMBER: 5830

SUBJECT'S LAST NAME:

VERIFICATION OF CAL

SUBJECT'S FIRST NAME/MI :

U

O.L. #: 1

DEPT/AGENCY: CNTB

CASE/REPORT: 1

TEST TYPE: U

ALCO TARGET VALUE: .000

ALCO S/N: 130578 *BMB*  
58442 3/6/11

--- BREATH ANALYSIS ---

.000 ADJUSTED FOR 26.9% in		
ALCO TARGET	.072	15:00
BLANK TEST	.000	15:02
INTERNAL STANDARD	VERIFIED	15:02
ALCO TV 26.9% in	.074	15:02
BLANK TEST	.000	15:03
SUBJECT SAMPLE	.000	15:03
BLANK TEST	.000	15:04
ALCO TV 26.9% in	.074	15:04
BLANK TEST	.000	15:05

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130128

JANUARY 25, 2011

TIME 14:46

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY

PROGRAM: OKAY

SOFTWARE DATE: 01/08/09

HEATERS

SAMPLE CHAMBER: 49c

BREATH TUBE: 43c

BAROMETER: 26.96 in

FLOW DETECTOR: OKAY

PUMP

HIGH SPEED: OKAY

DETECTOR: OKAY

FILTERS: OKAY

QUARTZ STANDARD: OKAY

CALIBRATION: OKAY

PRINTER TEST

!@#%&'()\*+,-./0123456789:;=<?@ABCDEF6  
HIJKLMNOPQRSTUVWXYZ[\]^\_`abcdefgijklmnop  
qrstuvwxyzi)-||