

# VERIFICATION OF CALIBRATION REPORT

of Datamaster cdm

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

JAN 20 2010

Supervisor/Operator Performing the Verification Procedure:		Datamaster cdm S/N <u>130131</u>	
Name <u>Shayne Calt</u>		ID# <u>4559</u>	Date <u>1-15-10</u>
A	Agency <u>AST</u>	Phone # <u>733-2256</u>	
Instrument Location <u>Talkeetna AST</u>			
Alco S/N <u>31343</u>		Target Value <u>.084</u>	High Pressure <u>500</u>
B	Alco Test Value Average <u>.080</u>		<u>.080</u>
	1 <sup>st</sup> Alco	2 <sup>nd</sup> Alco	
Signature <u>[Signature]</u>		<u>CUB</u> <u>1/20/10</u>	
(OVER)			

(Do Not write in the area below)


I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

[Signature]  
Nita J. Bolz  
Scientific Director  
State Breath Alcohol Program

Subscribed and sworn before me this 20<sup>th</sup> day of January, 2010.

[Signature] (Notary Seal Stamp)  
Carolyn M. Noland  
Notary Public, State of Alaska  
Commission Expires with Office

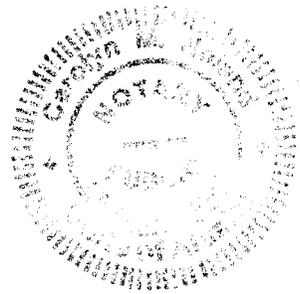

# VERIFICATION OF CALIBRATION REPORT

of Datamaster cdm

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Datamaster cdm S/N 130131

(CONTINUED FROM FRONT PAGE)

**C** TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130131

JANUARY 15, 2010 *(AS 1122110)*

OPERATOR'S NAME:  
GALT SHAYNE M

OPERATOR'S NUMBER: 4559

SUBJECT'S LAST NAME:  
VERIFICATION OF CAL

SUBJECT'S FIRST NAME/MI :  
U

O.L. #: U

DEPT/AGENCY: TAL0

CASE/REPORT: U

TEST TYPE: U

ALCO TARGET VALUE: .004

ALCO S/N: 31343

--- BREATH ANALYSIS ---

.004 ADJUSTED FOR 28.90 in		
ALCO TARGET	.001	15:17
BLANK TEST	.000	15:18
INTERNAL STANDARD	VERIFIED	15:18
ALCO TU 28.90 in	.000	15:18
BLANK TEST	.000	15:19
SUBJECT SAMPLE <i>(AS 1122110)</i>	.000	15:19
BLANK TEST	.000	15:20
ALCO TU 28.90 in	.000	15:21
BLANK TEST	.000	15:21

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130131

JANUARY 15, 2010  
TIME 15:15

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY

PROGRAM: OKAY

SOFTWARE DATE: 02/20/01

HEATERS

SAMPLE CHAMBER: 50c

BREATH TUBE: 43c

BAROMETER: 28.90 in

FLOW DETECTOR: OKAY

PUMP

HIGH SPEED: OKAY

DETECTOR: OKAY

FILTERS: OKAY

QUARTZ STANDARD: OKAY

CALIBRATION: OKAY

PRINTER TEST

!\*"#%&'()\*+,-./0123456789:;<=>?@ABCDEF6  
HIJKL MNOPQRSTU VWXYZ[\]^\_`ab cde fghijklmno  
pqrstu vwxyz{|}~