

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

DEC 29 2010

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	<u>130134</u> ✓
Name		<u>Tyron Walker</u>	ID# <u>4535</u> ✓ Date <u>12/24/10</u> ✓
A	Agency	<u>Ketchikan Police Dept.</u>	Phone # <u>225-6631</u>
Instrument Location		<u>301 Main St.</u>	<u>Ketchikan AK</u>
Alco S/N		<u>70729</u> ✓	Target Value <u>.084</u> ✓ High Pressure <u>900</u>
B	Alco Test Values	<u>.086</u> ✓ 1st Alco	<u>.085</u> ✓ 2 nd Alco
Signature		<u>Tyron Walker</u>	<u>CB</u> <u>12/29/10</u>

(OVER)

(Do Not write in the area below)



I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

Nita J. Bolz
Nita J. Bolz
Scientific Director
State Breath Alcohol Program

Subscribed and sworn before me this 11th day of FEB, 2011 PM

Daniel L. Nicholas
(Notary Seal Stamp)
Daniel L. Nicholas
Notary Public, State of Alaska
Commission Expires with Office

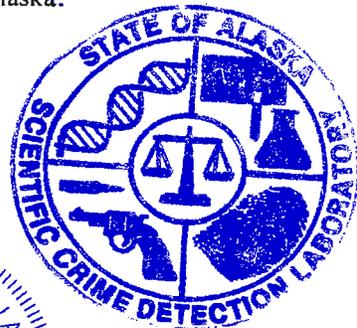

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N

130134

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130134

DECEMBER 24, 2010 COB 12/30/10

OPERATOR'S NAME:
WALKER TY
OPERATOR'S NUMBER: 4555
SUBJECT'S LAST NAME:
VERIFICATION OF CAL
SUBJECT'S FIRST NAME/MI :

T
O.L. #: 12345
DEPT/AGENCY: KETI
CASE/REPORT: 10-1234
TEST TYPE: U
ALCO TARGET VALUE: .004
ALCO S/N: 70729

--- BREATH ANALYSIS ---

.004 ADJUSTED FOR 29.65 in
ALCO TARGET .003 21:30
BLANK TEST .000 21:31
INTERNAL STANDARD VERIFIED 21:32
ALCO TV 29.65 in .006 21:32
BLANK TEST .000 21:33
SUBJECT SAMPLE .000 21:33
BLANK TEST .000 21:34
ALCO TV 29.65 in .005 21:34
BLANK TEST .000 21:35

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130134

DECEMBER 24, 2010
TIME 21:36

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY
PROGRAM: OKAY
SOFTWARE DATE: 01/08/09
HEATERS
SAMPLE CHAMBER: 48c
BREATH TUBE: 41c
BAROMETER: 29.65 in
FLOW DETECTOR: OKAY
PUMP
HIGH SPEED: OKAY
DETECTOR: OKAY
FILTERS: OKAY
QUARTZ STANDARD: OKAY
CALIBRATION: OKAY

PRINTER TEST

!@#%&'()*+,-./0123456789:;<=>?@ABCDEF
HIJKLMNPORS TUUVWXYZ[\]^_`abcde fghi jklmno
pqrstuvwxyz{|}~