

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N: 130135

Supervisor/Operator Performing the Verification Procedure:

Name: Trp. J. Santora ID# 2276 Date: 1-26-2012

A

Agency: Alaska State Troopers Phone # 656-1233

Instrument Location: Galena Police Department

B

Alco S/N: 78855 Target Value: .081 High Pressure: 650

Alco Test Values .081 .081

1st Alco

2nd Alco

Signature


(OVER)

CRF 1/31/12

(Do Not write in the area below)

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:


- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

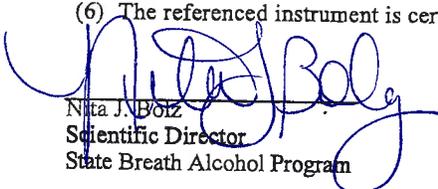
Nita J. Bolz
Scientific Director
State Breath Alcohol Program

Subscribed and sworn before me this 2nd day of Feb 2012.

 (Notary Seal Stamp)

~~AND~~ Daniel L. Nicholas
Notary Public, State of Alaska
Commission Expires with Office



VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130135

(CONTINUED FROM FRONT PAGE)

C

TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130135

JANUARY 26, 2012

OPERATOR'S NAME:

SANTORA JEANNINE L

OPERATOR'S NUMBER: 2276

SUBJECT'S LAST NAME:

VERIFICATION

SUBJECT'S FIRST NAME/MI:

OF CAL

O.L. #: 0000000

DEPT/AGENCY: GALA

CASE/REPORT:

TEST TYPE: V

ALCO TARGET VALUE: .081

ALCO S/N: 78855

--- BREATH ANALYSIS ---

.081 ADJUSTED FOR 30.07 in		
ALCO TARGET	.081	10:29
BLANK TEST	.000	10:31
INTERNAL STANDARD	VERIFIED	10:31
ALCO TV 30.07 in	.081	10:31
BLANK TEST	.000	10:32
SUBJECT SAMPLE	.000	10:33
BLANK TEST	.000	10:33
ALCO TV 30.07 in	.081	10:34
BLANK TEST	.000	10:35

CRF 1/31/12

CRF 1/31/12

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130135

JANUARY 26, 2012

TIME 10:35

--- DIAGNOSTIC CHECK ---

COMPUTER:	OKAY
PROGRAM:	OKAY
SOFTWARE DATE:	02/20/01
HEATERS	
SAMPLE CHAMBER:	48c
BREATH TUBE:	43c
BAROMETER:	30.07 in
FLOW DETECTOR:	OKAY
PUMP	
HIGH SPEED:	OKAY
DETECTOR:	OKAY
FILTERS:	OKAY
QUARTZ STANDARD:	OKAY
CALIBRATION:	OKAY

PRINTER TEST

!@#%&'()*+,-./0123456789:;<=>?@BCDEF6
HIJKL;NOPQRSTUWXYZ\]^_`'abcde fghijklmno
pqrs tuvwxyz{|}~