

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N: 130135

Supervisor/Operator Performing the Verification Procedure:

Name: Trp. J. Santora ID# 2276 Date: 7-4-12

A Agency: Alaska State Troopers Phone # 656-1233

Instrument Location: Galena Police Department

B Alco S/N: 78855 Target Value: .081 High Pressure: 600

Alco Test Values .080 .079  
1<sup>st</sup> Alco 2<sup>nd</sup> Alco

Signature

(OVER)

BMB  
7/9/12

(Do Not write in the area below)



I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

Nita J. Bolz  
Scientific Director  
State Breath Alcohol Program

Subscribed and sworn before me this 20<sup>th</sup> day of July, 2012. NAAC 7/20/12

Nikki Roth (Notary Seal Stamp)  
Daniel L. Nicholas NIKKI ROTH 7/20/12  
Notary Public, State of Alaska  
Commission Expires with Office

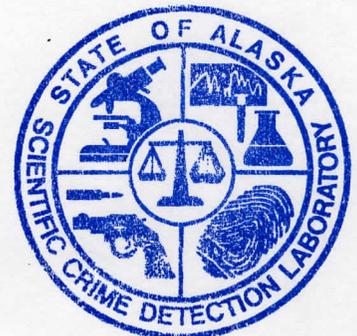

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130135

(CONTINUED FROM FRONT PAGE)

**C** TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130135

JULY 04, 2012

*BMB 7/9/12*

OPERATOR'S NAME:  
SANTORA JEANNINE L  
OPERATOR'S NUMBER: 2276  
SUBJECT'S LAST NAME:  
VERIFICATION  
SUBJECT'S FIRST NAME/MI :  
OF CAL  
O.L. #: 0000000  
DEPT/AGENCY: GALO  
CASE/REPORT:  
TEST TYPE: U  
ALCO TARGET VALUE: .061  
ALCO S/N: 78855

--- BREATH ANALYSIS ---

.061 ADJUSTED FOR 29.90 in		
ALCO TARGET	.060	14:29
BLANK TEST	.000	14:30
INTERNAL STANDARD	VERIFIED	14:30
ALCO TV 29.90 in	.060	14:31
BLANK TEST	.000	14:31
SUBJECT SAMPLE	.060	14:32
BLANK TEST	.000	14:33
ALCO TV 29.90 in	.079	14:33
BLANK TEST	.000	14:34

*BMB 7/9/12*

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130135

JULY 04, 2012  
TIME 14:36

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY  
PROGRAM: OKAY  
SOFTWARE DATE: 02/20/01

HEATERS  
SAMPLE CHAMBER: 49c  
BREATH TUBE: 42c

BAROMETER: 29.90 in

FLOW DETECTOR: OKAY

PUMP  
HIGH SPEED: OKAY

DETECTOR: OKAY

FILTERS: OKAY

QUARTZ STANDARD: OKAY

CALIBRATION: OKAY

PRINTER TEST  
!"#\$%&'()\*+,-./0123456789:;<=;>@ABCDEFGHIJKL  
MNOPQRSTUVWXYZ[\]^\_`abcde fghi jk lano  
pqrs tuvwxyz{|}~