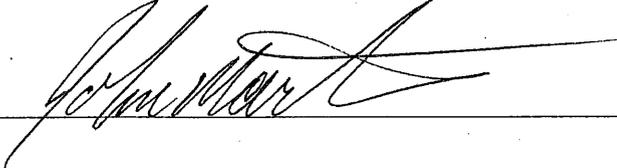


VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	<u>130142</u> ✓
Name	<u>John Martin</u>	ID#	<u>6101</u>
		Date	<u>20 February 08</u>
A	Agency	<u>Directorate of Emergency Services, FRN4</u>	Phone # <u>384-3883</u>
	Instrument Location	<u>Bldg #656 A Street FT Richardson, AK 99505</u>	
B	Alco S/N	<u>78820</u> ✓	Target Value <u>.080</u> ✓
		High Pressure	<u>1150</u>
	Alco Test Values	<u>.079</u>	<u>.078</u>
		1 st Alco	2 nd Alco
	Signature		
		(OVER)	<u>008</u> <u>3/11/08</u>


(Do Not write in the area below)

Under the Alaska Rules of Evidence, I certify that;


(a) I am Jeanne Swartz, Forensic Scientist III, Scientific Crime Detection Laboratory, State of Alaska Department of Public Safety, and was, at the time of signing, the custodian of the records of the aforementioned laboratory and the signature was made in my official capacity as Scientific Director Designee of the State Breath Alcohol Testing Program.

(b) The verification of calibration for the above instrument has been received and reviewed. Instrument operator, John Martin, whose name appears in my records, is qualified to verify the calibration of the above instrument.

(c) This instrument is certified for evidentiary use and these records are being retained as original documents in my custody.

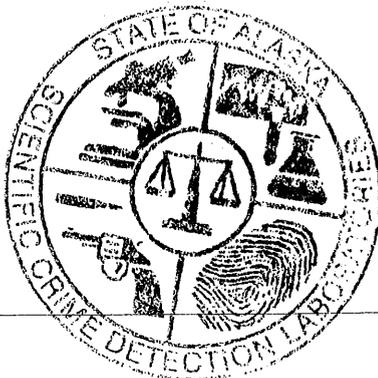

Signed and sealed



Jeanne Swartz
Scientific Director Designee
State of Alaska
State Breath Alcohol Testing Program

3/12/08
Date

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130142

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130142

FEBRUARY 20, 2000

OPERATOR'S NAME:

MARTIN/JOHN/B

OPERATOR'S NUMBER: 6101

SUBJECT'S LAST NAME:

VERIFICATION OF CAL

SUBJECT'S FIRST NAME/NI :

NA

O.L. #: NA

DEPT/AGENCY: FRM

CASE/REPORT: NA

TEST TYPE: U

ALCO TARGET VALUE: .000

ALCO S/N: 78820

--- BREATH ANALYSIS ---

.000 ADJUSTED FOR 29.25 in

ALCO TARGET	.078	09:11
BLANK TEST	.000	09:12
INTERNAL STANDARD	VERIFIED	09:12
ALCO TV 29.26 in	.079	09:13
BLANK TEST	.000	09:14
SUBJECT SAMPLE	.000	09:14
BLANK TEST	.000	09:15
ALCO TV 29.26 in	.078	09:16
BLANK TEST	.000	09:16

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130142

FEBRUARY 20, 2000

TIME 09:17

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY

PROGRAM: OKAY

SOFTWARE DATE: 03/29/00

HEATERS

SAMPLE CHAMBER: 43c

BREATH TUBE: 44c

BAROMETER: 29.26 in

FLOW DETECTOR: OKAY

PUMP

HIGH SPEED: OKAY

DETECTOR: OKAY

FILTERS: OKAY

QUARTZ STANDARD: OKAY

CALIBRATION: OKAY

PRINTER TEST

!#\$%&'()*+,-./0123456789:;<=>?@ABCDEF6
HIJKLMNPOQRSTUVWXYZ[\]^_`abcdefg h i j k l m n o
p q r s t u v w x y z { } ~ |